


User Manual
English

Stratos Pro A2.. MSOxy Oxygen Measurement with Memosens Sensors

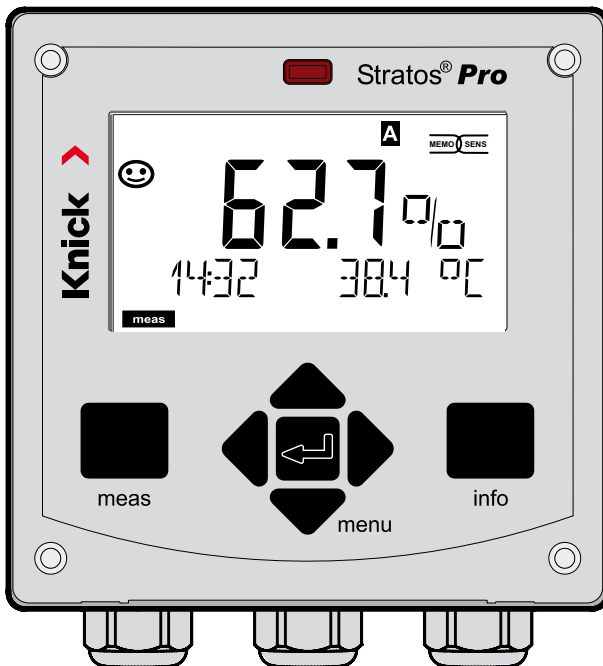

About This Manual.

Return of products

Please contact our Service Team before returning a defective device. Ship the cleaned device to the address you have been given. If the device has been in contact with process fluids, it must be decontaminated/disinfected before shipment. In that case, please attach a corresponding certificate, for the health and safety of our service personnel.

Disposal


Please observe the applicable local or national regulations concerning the disposal of “waste electrical and electronic equipment”.

About this manual:

This manual is intended as a reference guide to your device – You don't have to read the book from front to back.

Take a look at the **Table of Contents** or the **Index** to find the function you are interested in. Each topic is explained on a double-page spread with step-by-step instructions on how to configure the desired function. Clearly legible page numbers and headlines help you to quickly find the information:

Left page:
How do I get to the function

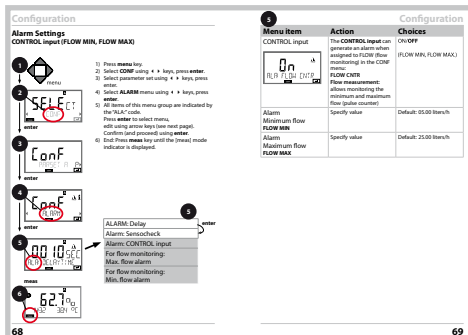

Right page:
Which settings are provided for this function

Safety Instructions

In official EU languages and others

Quickstart Guides

Installation and first steps:

- Operation
- Menu structure
- Calibration
- Error messages and recommended actions

Specific Test Report

Electronic Documentation

Manuals + Software

Ex Devices:

Control Drawings

EU Declarations of Conformity

Up-to date documentation available on our website:



www.knick.de

Contents

Documents Supplied	3
Introduction	7
Intended Use	7
Safety Information	10
Overview of Stratos Pro A2... MSOXY	11
Assembly	12
Package Contents	12
Mounting Plan, Dimensions	13
Pipe Mounting, Protective Hood.....	14
Panel Mounting	15
Installation	16
Installation Instructions.....	16
Rating Plates / Terminal Assignments.....	16
Wiring of Stratos Pro A2... MSOXY	17
Memosens Cable: Wire Colors.....	18
Wiring Example.....	19
Connecting a Memosens Sensor	20
User Interface, Keypad	21
Display	22
Signal Colors (Display Backlighting)	22
Measuring Mode.....	23
Selecting the Mode / Entering Values.....	24
Color-Coded User Interface	26
Operating Modes.....	27
Menu Structure of Modes and Functions	28
HOLD Mode	29
Alarm	30
Alarm and HOLD Messages.....	31
Configuration	32
Menu Structure of Configuration.....	32
Manual Switchover of Parameter Sets A/B.....	34
Parameter Sets (Original for Copy)	42

Sensor.....	44
Sensor Verification (TAG, GROUP).....	52
Current Output 1.....	54
Current Output 2.....	62
Correction.....	64
CONTROL Input.....	66
Alarm.....	68
Time and Date.....	72
Measuring Points (TAG/GROUP).....	72
Digital Sensors.....	74
Memosens Sensors:	
Calibration and Maintenance in the Lab.....	74
Memosens Sensors: Configuring the Device.....	75
Replacing a Sensor.....	76
Calibration.....	78
Selecting a Calibration Mode.....	79
Zero Calibration.....	80
Product Calibration.....	82
Slope Calibration (Medium: Water).....	84
Slope Calibration (Medium: Air).....	85
Temp Probe Adjustment.....	86
Measurement.....	87
Diagnostics.....	88
Service.....	93
Operating States.....	96
A2...X: Supply Units and Connection.....	97
Product Line and Accessories.....	98
Specifications.....	99
Error Handling.....	104
Error Messages.....	105
Sensoface.....	108

Contents

FDA 21 CFR Part 11	111
Electronic Signature – Passcodes.....	111
Audit Trail.....	111
Index	112
Trademarks.....	119
Passcodes	120

Intended Use

Stratos Pro A2... MSOXY is a 2-wire device for dissolved oxygen and temperature measurement using Memosens sensors in biotechnology, pharmaceutical industry, as well as in the field of industry, environment, food processing and sewage treatment. Optionally, it can be used for measuring oxygen traces.

Enclosure and mounting possibilities

- The sturdy molded enclosure is rated IP 67/NEMA 4X for outdoor use. It is made of glass-reinforced PBT / PC and measures 148 mm x 148 mm x 117 mm (H x W x D). It is provided with knockouts to allow:
 - wall mounting (with sealing plugs to seal the enclosure), see page 13
 - post/pipe mounting (Ø 40 ... 60 mm, □ 30 ... 45 mm) see page 14
 - panel mounting (138 mm x 138 mm cutout to DIN 43700), see page 15

Weather protector (accessory)

The weather protector, which is available as accessory, provides additional protection against direct weather exposure and mechanical damage, see page 14.

Connection of sensors, cable glands

For connecting the cables, the enclosure provides

- 3 knockouts for cable glands M20x1.5
- 2 knockouts for NPT 1/2" or rigid metallic conduit

For quasi-stationary installations with Memosens sensors, we recommend using the M12 device socket (accessory ZU 0822) instead of a cable gland – it allows simple replacement of the sensor cable without opening the device.

Sensors

The device has been designed for Memosens standard sensors or Memosens trace sensors (optional).

Introduction

Display

Plain-text messages in a large, backlit LC display allow intuitive operation. You can specify which values are to be displayed in standard measuring mode ("Main Display", see page 25).

Color-coded user interface

The colored display backlighting signals different operating states (e.g. alarm: red, HOLD mode: orange, see page 26).

Diagnostics functions

"Sensocheck" and "Sensoface" monitor the sensor and provide clear information about its status, see page 108.

Data logger

The internal logbook (TAN SW-A002) can handle up to 100 entries – up to 200 with AuditTrail (TAN SW-A003), see page 91.

2 parameter sets A/B

The device provides two parameter sets which can be switched manually or via a control input for different process adaptations or different process conditions.

For overview of parameter sets (table for copy), see page 42.


Password protection

Password protection (passcodes) for granting access rights during operation can be configured, see page 95.

Correction

Here, you can adapt the device to the process conditions by means of salinity and pressure correction, either manually or via an external current input (optional, released by TAN), see page 64.

Control inputs

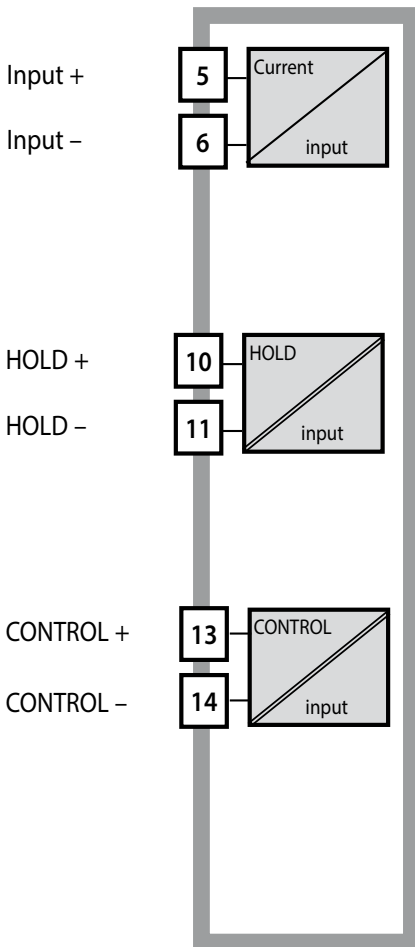

I input

The analog (0) 4 ... 20 mA current input can be used for external pressure compensation (TAN required). See page 64.

HOLD

(floating digital control input)
The HOLD input can be used for external activation of the HOLD mode, see page 30.

CONTROL

(floating digital control input)
The CONTROL input can be used either for parameter set selection (A/B) or for flow monitoring, see page 66.

Signal outputs

The device provides two current outputs (for transmission of measured value and temperature, for example).

Options

Additional functions can be activated by entering a TAN (page 95).

Safety Information

Safety Information

Be sure to read and observe the following instructions!

The device has been manufactured using state of the art technology and it complies with applicable safety regulations.

When operating the device, certain conditions may nevertheless lead to danger for the operator or damage to the device.



When using the device in a hazardous location, observe the specifications of the Control Drawing.



CAUTION!

Commissioning must only be performed by trained personnel authorized by the operating company! Whenever it is likely that protection has been impaired, the device shall be made inoperative and secured against unintended operation.

The protection is likely to be impaired if, for example:


- the device shows visible damage
- the device fails to perform the intended measurements
- after prolonged storage at temperatures below $-30\text{ }^{\circ}\text{C}$ / $-22\text{ }^{\circ}\text{F}$ or above $+70\text{ }^{\circ}\text{C}$ / $+158\text{ }^{\circ}\text{F}$
- after severe transport stresses

Before recommissioning the device, a professional routine test must be performed. This test must be carried out at the manufacturer's factory.

Note:

Before commissioning you must prove that the device may be connected with other equipment.

Overview of Stratos Pro A2... MSOXY

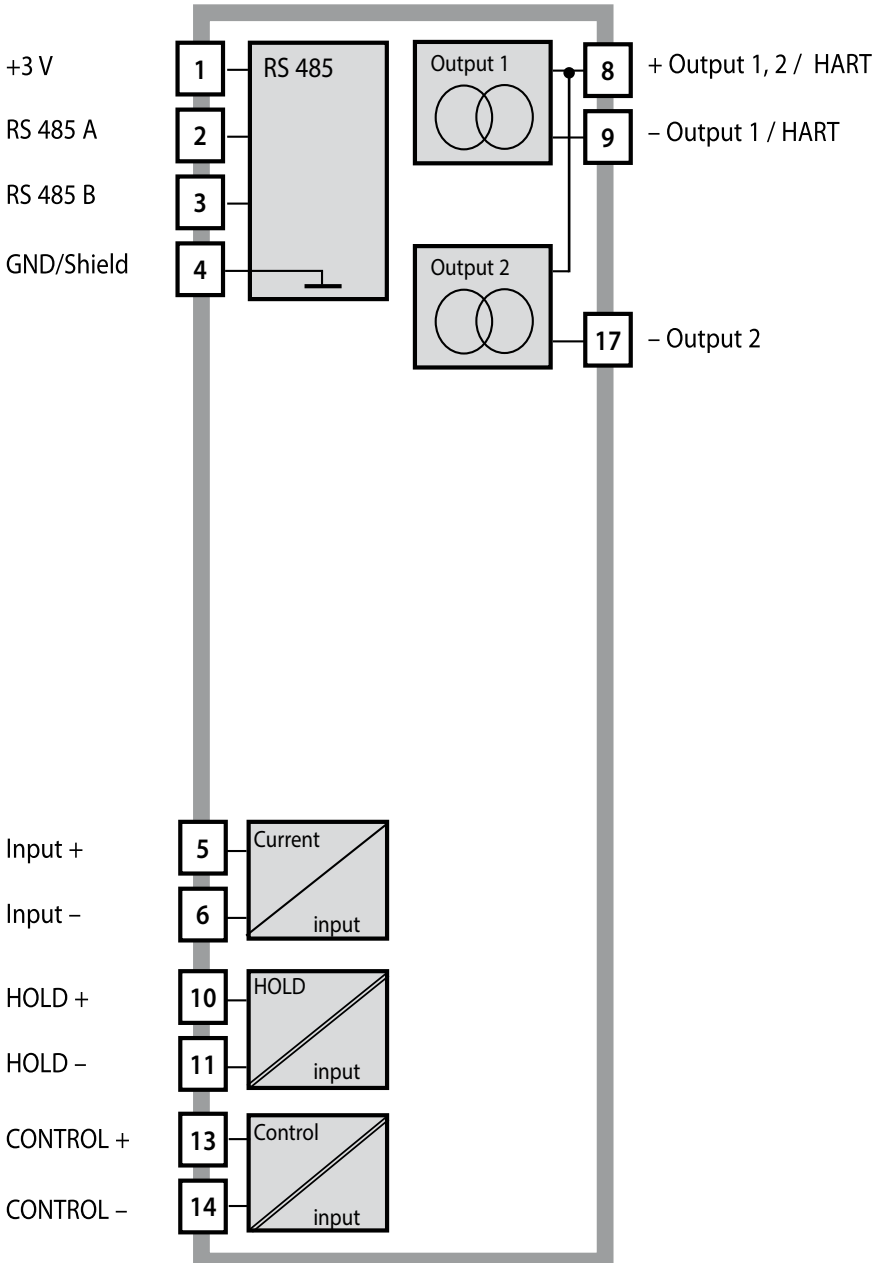

Assembly

Package Contents

Check the shipment for transport damage and completeness!

The package should contain:

- Front unit, rear unit, bag containing small parts
- Specific test report
- Documentation (cf p. 3)

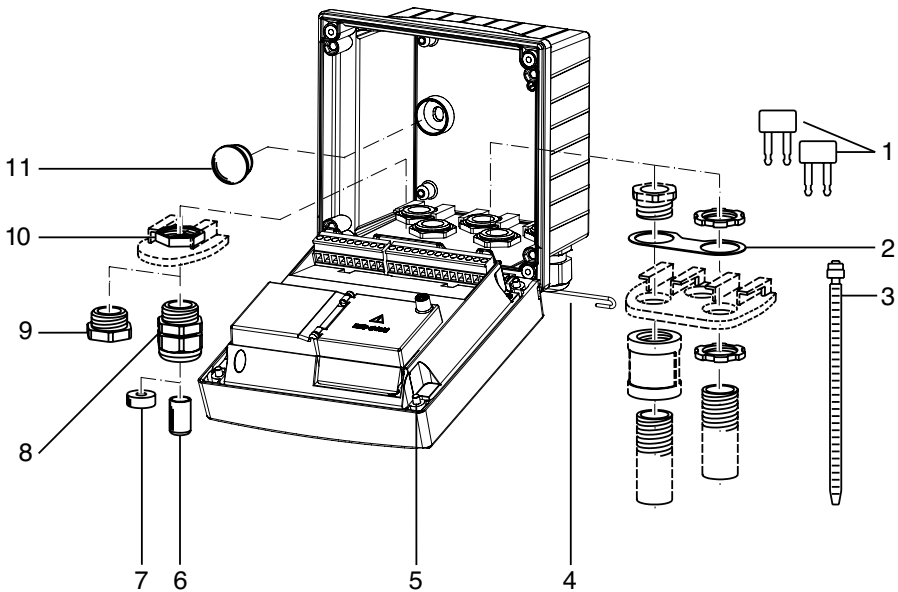


Fig.: Assembling the enclosure

- | | |
|---|--|
| 1) Jumper (3 x) | 6) Sealing insert (1 x) |
| 2) Washer (1 x), for conduit mounting: Place washer between enclosure and nut | 7) Rubber reducer (1 x) |
| 3) Cable tie (3 x) | 8) Cable gland (3 x) |
| 4) Hinge pin (1 x), insertable from either side | 9) Filler plug (3 x) |
| 5) Enclosure screw (4 x) | 10) Hexagon nut (5 x) |
| | 11) Sealing plug (2 x), for sealing in case of wall mounting |

Mounting Plan, Dimensions


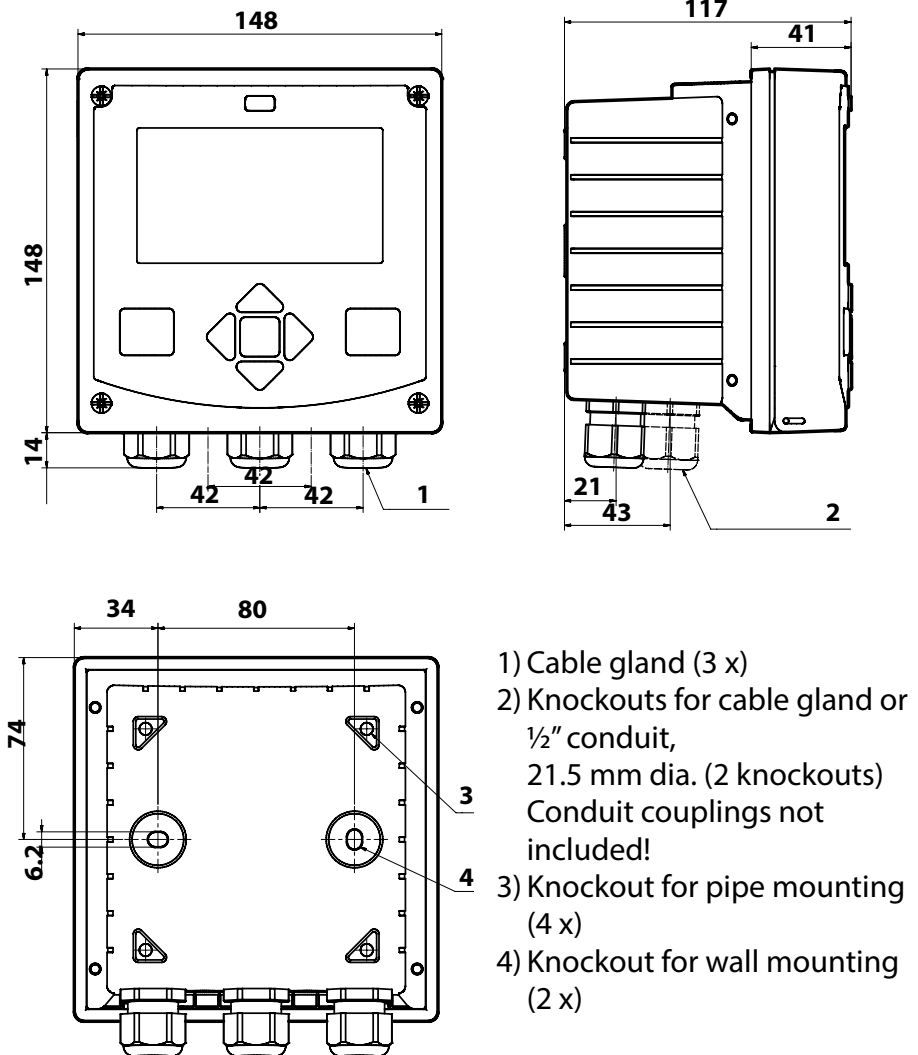


Fig.: Mounting plan (All dimensions in mm!)

Pipe Mounting, Protective Hood

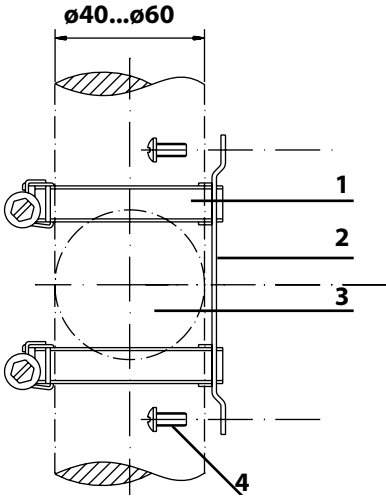

- 1) Hose clamp with worm gear drive to DIN 3017 (2 x)
- 2) Pipe-mount plate (1 x)
- 3) For vertical or horizontal posts or pipes
- 4) Self-tapping screw (4 x)

Fig.: Pipe-mount kit, accessory ZU 0274 (All dimensions in mm!)


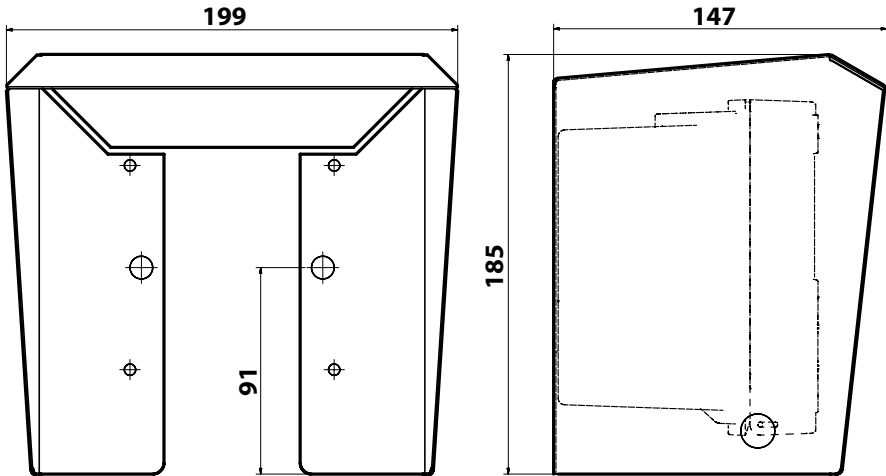


Fig.: Protective hood for wall and pipe mounting, accessory ZU 0737 (All dimensions in mm!)

Panel Mounting

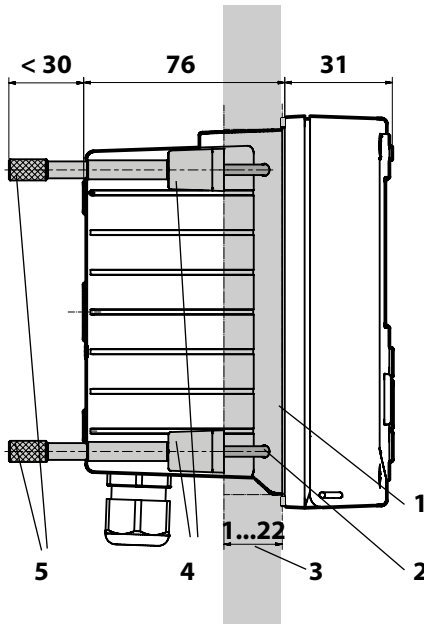

- 1) Circumferential sealing (1 x)
- 2) Screws (4 x)
- 3) Position of control panel
- 4) Span piece (4 x)
- 5) Threaded sleeve (4 x)

Cutout
138 x 138 mm (DIN 43700)

Fig.: Panel-mount kit, accessory ZU 0738 (All dimensions in mm!)

Installation

Installation Instructions

- Installation of the device must be carried out by trained experts in accordance with this user manual and as per applicable local and national codes.
- Be sure to observe the technical specifications and input ratings during installation!
- Be sure not to notch the conductor when stripping the insulation!
- The supplied current must be galvanically isolated. If not, connect an isolator module.
- All parameters must be set by a system administrator prior to commissioning!

Terminals:

suitable for single wires / flexible leads up to 2.5 mm² (AWG 14)

Rating Plates / Terminal Assignments

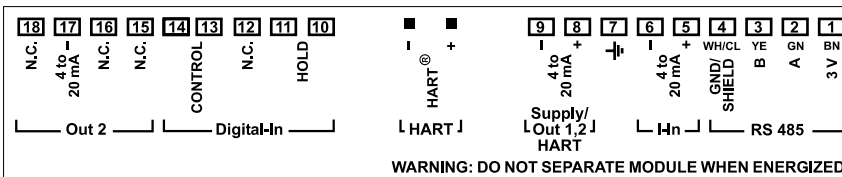


Fig.: Terminal assignments of Stratos Pro A2...


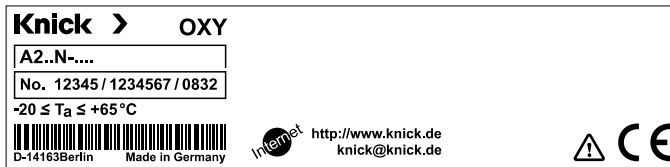


Fig.: Stratos Pro A2...N rating plate at outside bottom of front

Wiring of Stratos Pro A2... MSOXY

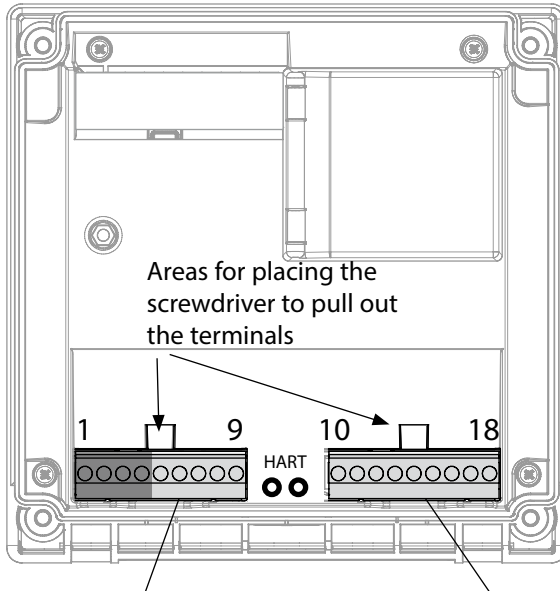

Terminal row 1		
1 (BN)	+3 V	⚠
2 (GN)	RS 485 A	⚠
3 (YE)	RS 485 B	⚠
4 (WH)	GND/shield	⚠
5	+ input	
6	- input	
7	PA	
8	+out 1,2/HART	
9	- out 1/HART	

Terminal row 2	
10	hold
11	hold
12	n.c.
13	contr
14	contr
15	n.c.
16	n.c.
17	- out 2
18	n.c.


In addition:

2 HART pins (between terminal row 1 and 2)

⚠ Sensor connection: RS-485 for Memosens


Fig.: Terminals, device opened, back of front unit

Memosens Cable: Wire Colors

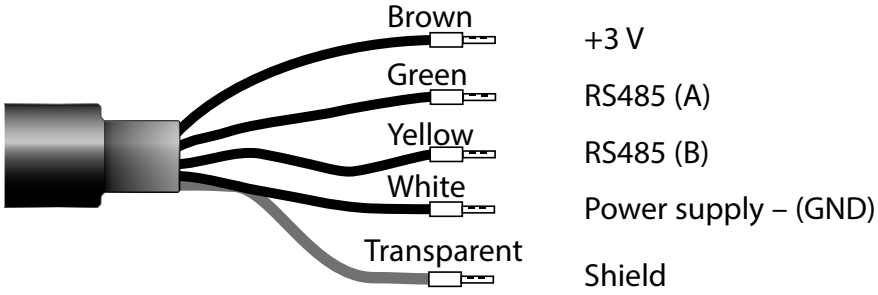


Wiring Example

Measuring task: Oxygen (standard)
Sensors (example): SE 706-NMSN (Knick)
Cable (example): CA/MS-003NAA (Knick)

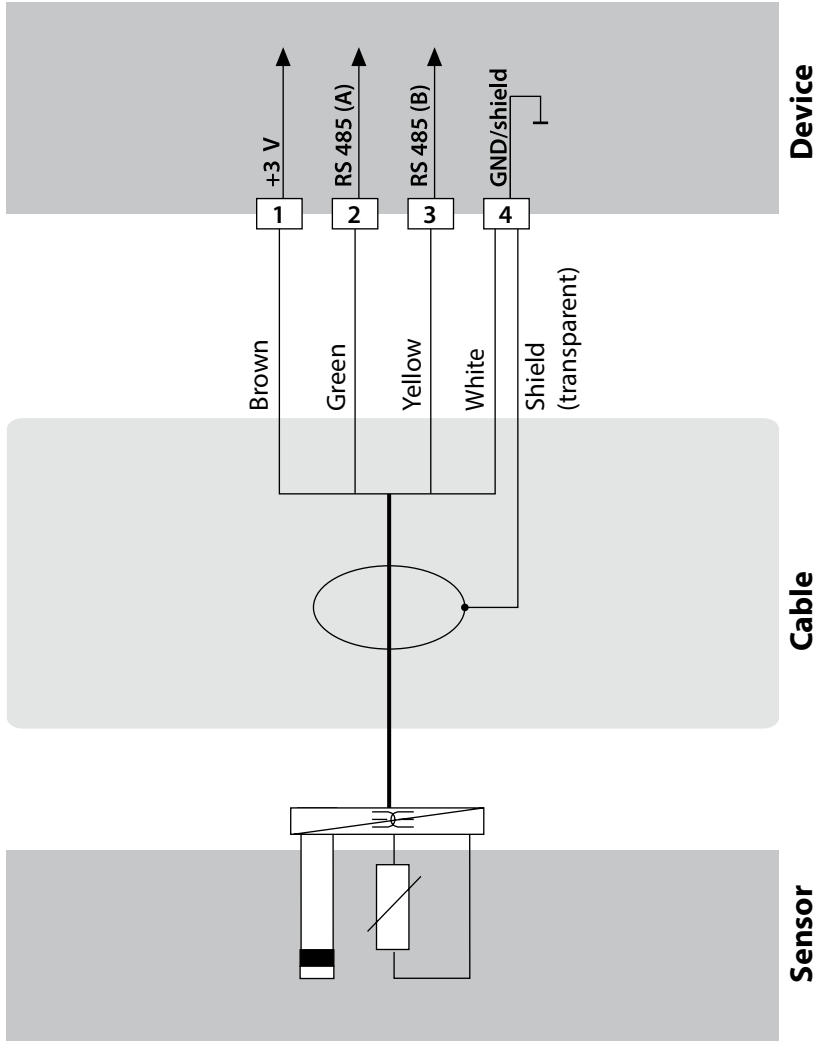

Connecting a Memosens Sensor

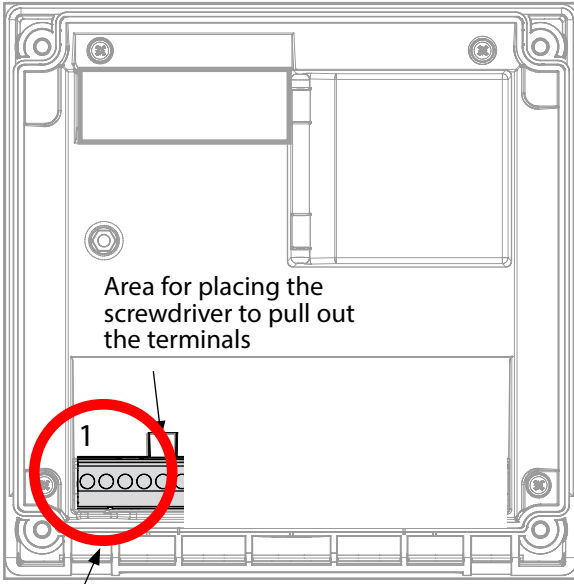


Memosens connection:		Wire color
1	+3 V	Brown
2	RS 485 A	Green
3	RS 485 B	Yellow
4	GND/shield	White, transparent shield

Connect the Memosens sensor to the RS-485 interface of the device using the Memosens cable CA/MS.... . When the sensor is selected in the Configuration menu, the default values are taken as calibration data. They can then be modified by calibration.




NOTICE!
The measuring module slot must be empty!
Stratos Pro A2... MSOxy is intended for connecting a Memosens sensor via RS-485 interface. It does not provide a measuring module.

User Interface, Keypad

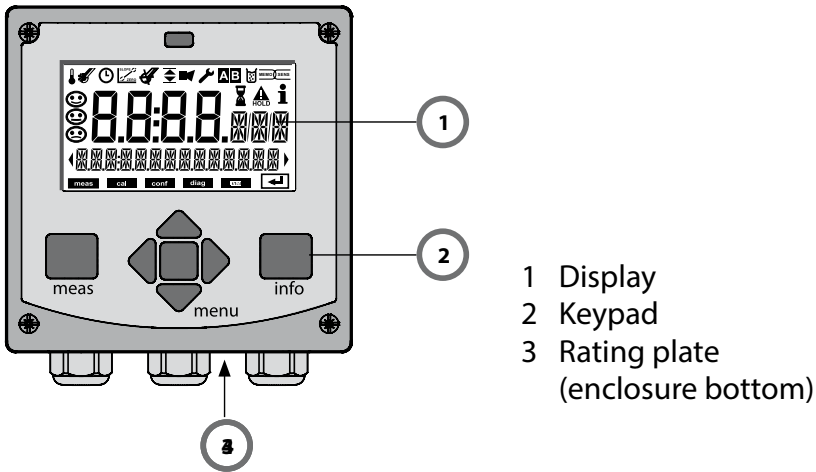

Key	Function
meas	<ul style="list-style-type: none">• Return to last menu level• Directly to measuring mode (press > 2 s)• Measuring mode: other display
info	<ul style="list-style-type: none">• Retrieve information• Show error messages
enter	<ul style="list-style-type: none">• Configuration: Confirm entries, next configuration step• Calibration: Continue program flow
menu	<ul style="list-style-type: none">• Measuring mode: Call menu
Arrow keys up / down	<ul style="list-style-type: none">• Menu: Increase/decrease a numeral• Menu: Selection
Arrow keys left / right	<ul style="list-style-type: none">• Previous/next menu group• Number entry: Move between digits

Display

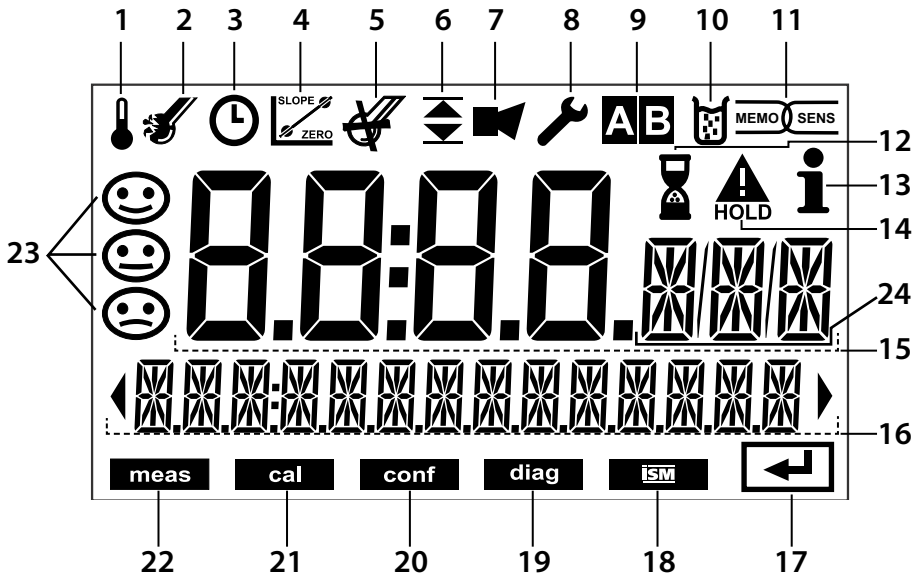


- | | | | |
|----|--|----|---------------------|
| 1 | Temperature | 13 | Info available |
| 2 | Sensocheck | 14 | Hold mode active |
| 3 | Interval/response time | 15 | Main display |
| 4 | Sensor data | 16 | Secondary display |
| 5 | Not used | 17 | Proceed using enter |
| 6 | Limit message:
Limit 1 ▼ or Limit 2 ▲ | 18 | ISM sensor |
| 7 | Alarm | 19 | Diagnostics |
| 8 | Service | 20 | Configuration mode |
| 9 | Parameter set | 21 | Calibration mode |
| 10 | Calibration | 22 | Measuring mode |
| 11 | Memosens sensor | 23 | Sensoface |
| 12 | Waiting time running | 24 | Unit symbols |

Signal Colors (Display Backlighting)

- | | |
|--------------|---|
| Red | Alarm (in case of fault: display values blink) |
| Red blinking | Input error: illegal value or wrong passcode |
| Orange | HOLD mode (Calibration, Configuration, Service) |
| Turquoise | Diagnostics |
| Green | Info |
| Magenta | Sensoface message |

Measuring Mode

After the operating voltage has been connected, the analyzer automatically goes to "Measuring" mode. To call the measuring mode from another operating mode (e.g. Diagnostics, Service): Hold **meas** key depressed (> 2 s).

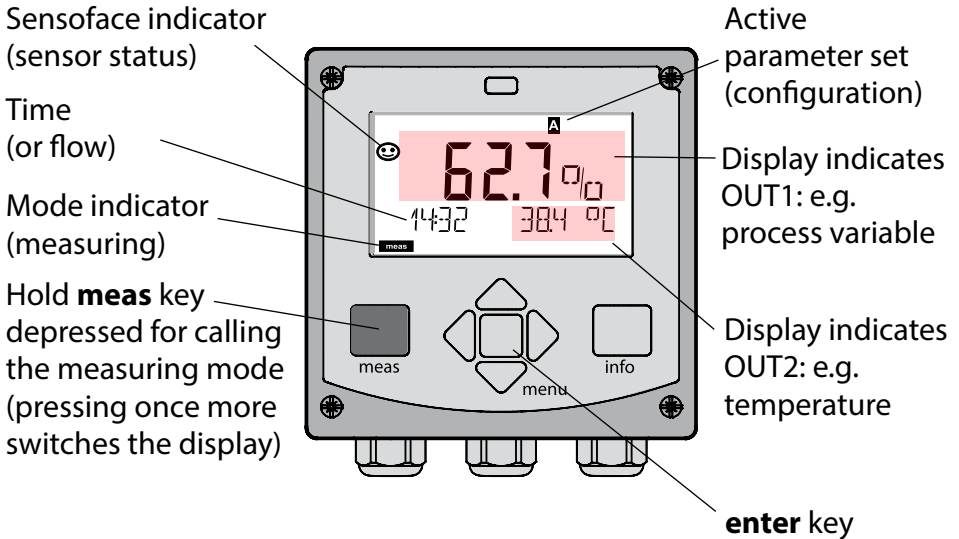

Depending on the configuration, one of the following displays can be set as standard display for the measuring mode (see page 25):

- Measured value, time and temperature (default setting)
- Measured value and selection of parameter set A/B or flow
- Measured value and tag number ("TAG")
- Time and date

Note: By pressing the **meas** key in measuring mode you can view the displays for approx. 60 sec.




The device must be configured for the respective measurement task!

Selecting the Mode / Entering Values


To select the operating mode:

- 1) Hold **meas** key depressed (> 2 s) (directly to measuring mode)
- 2) Press **menu** key: the selection menu appears
- 3) Select operating mode using left / right arrow key
- 4) Press **enter** to confirm the selected mode

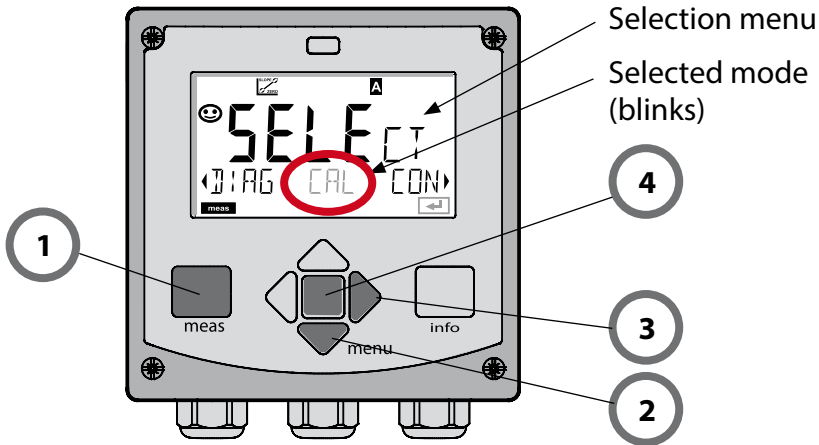


To enter a value:

- 5) Select numeral: left / right arrow key
- 6) Change numeral: up / down arrow key
- 7) Confirm entry by pressing **enter**

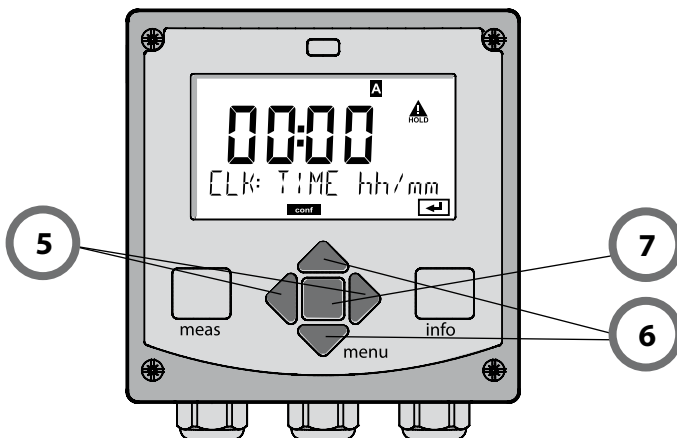


Display in Measuring Mode

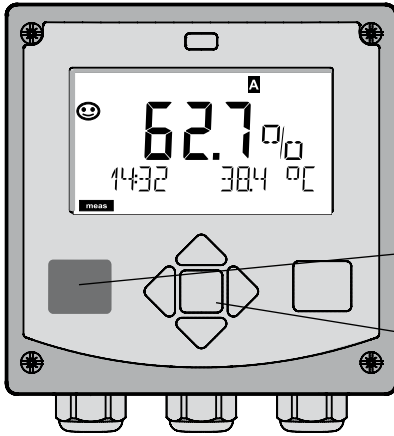



The MAIN DISPLAY is the display which is shown in measuring mode. To call the measuring mode from any other mode, hold the **meas** key depressed for at least 2 sec.

meas key


enter key



By pressing **meas** briefly you can step through further displays such as tag number (TAG) or flow (L/h). These displays are turquoise. After 60 sec they switch back to the main display.



Press **enter** to select a display as MAIN DISPLAY – the secondary display shows “MAIN DISPLAY – NO”. Use the **UP / DOWN** arrow keys to select “MAIN DISPLAY – YES” and confirm by pressing **enter**. The display color changes to white. This display is now shown in measuring mode.




Color-Coded User Interface


The color-coded user interface guarantees increased operating safety. Operating modes are clearly signaled.

The normal measuring mode is white. Information text appears on a green screen and the diagnostic menu appears on turquoise. The orange HOLD mode (e.g. during calibration) is quickly visible as is the magenta screen which indicates asset management messages for predictive diagnostics – such as maintenance request, pre-alarm and sensor wear.


The alarm status has a particularly noticeable red display color and is also signaled by flashing display values. Invalid inputs or false pass-codes cause the entire display to blink red so that operating errors are noticeably reduced.

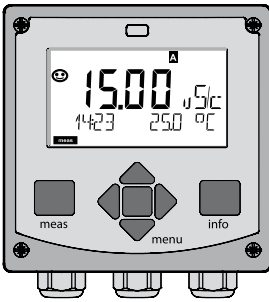


White:
Measuring mode

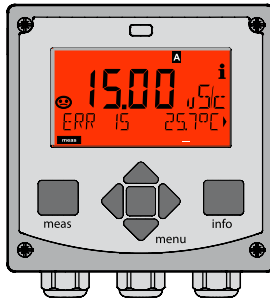


Red blinking:
Alarm, errors

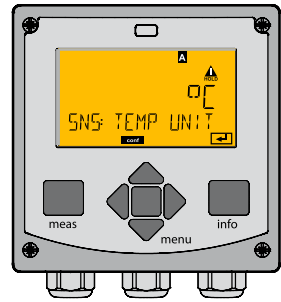


Orange:
HOLD mode

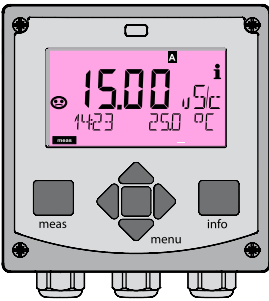

Magenta:
Maintenance request

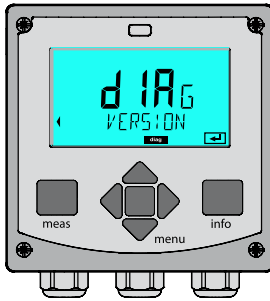

Turquoise:
Diagnostics

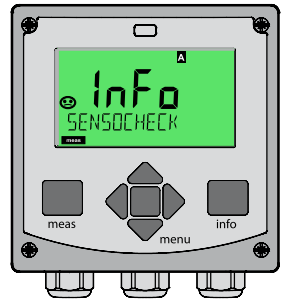

Green:
Information texts

Diagnostics

Display of calibration data, display of sensor data, performing a device self-test, viewing the logbook entries, display of hardware/software versions of the individual components. The logbook can store 100 events (00...99). They can be displayed directly on the device. The logbook can be extended to 200 entries using a TAN (Option).

HOLD

Manual activation of HOLD mode, e.g. for replacing a digital sensor. The signal outputs adopt a defined state.

Calibration

Every sensor has typical characteristic values, which change in the course of the operating time. Calibration is required to supply a correct measured value. The device checks which value the sensor delivers when measuring in a known solution. When there is a deviation, the device can be "adjusted". In that case, the device displays the "actual" value and internally corrects the measurement error of the sensor. Calibration must be repeated at regular intervals. The time between the calibration cycles depends on the load on the sensor. During calibration the device is in HOLD mode.

During calibration the device remains in the HOLD mode until it is stopped by the operator.

Configuration


The analyzer must be configured for the respective measurement task. In the "Configuration" mode you select the connected sensor, the measuring range to be transmitted, and the conditions for warning and alarm messages. During configuration the device is in HOLD mode.

Configuration mode is automatically exited 20 minutes after the last keystroke. The device returns to measuring mode.

Service

Maintenance functions (monitor, current source), passcode assignment, reset to factory settings, enabling of options (TAN).

Menu Structure of Modes and Functions



Pressing the **menu** key (down arrow) opens the selection menu. Select the menu group using the left/right arrow keys. Pressing **enter** opens a menu item. Press **meas** to return.



DIAG

CALDATA	Display of calibration data
SENSOR	Display of sensor data
SELFTEST	Self test: RAM, ROM, EEPROM, module
LOGBOOK	Logbook: 100 events with date and time
MONITOR	Display of direct, uncorrected sensor signals
VERSION	Display of software version, model designation, serial number

HOLD

Manual activation of HOLD mode, e.g. for sensor replacement. The signal outputs behave as configured (e.g. last measured value, 21 mA)

CAL

CAL_WTR/AIR	Calibration in water/air (as configured)
CAL_ZERO	Zero calibration
P_CAL	Product calibration
CAL_RTD	Adjustment of temperature probe

CONF

PARSET A	Configuring parameter set A
PARSET B	Configuring parameter set B

SERVICE

(Access via code, factory setting: 5555)

MONITOR	Display of measured values for validation (simulators)
SENSOR	Reset wear counter
OUT1	Current source, output 1
OUT2	Current source, output 2
CODES	Specifying access codes for operating modes
DEFAULT	Reset to factory setting
OPTION	Enabling an option via TAN

HOLD Mode

The HOLD mode is a safety state during configuration and calibration. Output current is frozen (LAST) or set to a fixed value (FIX). The HOLD mode is indicated by orange display backlighting.


HOLD mode, display icon:



Output signal response

- **LAST:** The output current is frozen at its last value. Recommended for short configuration procedures. The process should not change decisively during configuration. Changes are not noticed with this setting!
- **FIX:** The output current is set to a value that is noticeably different from the process value to signal the control system that the device is being worked at.

Output signal during HOLD:

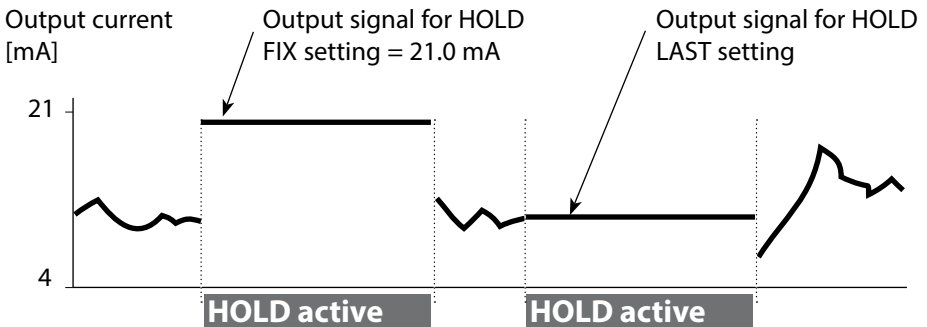

Terminating the HOLD mode


The HOLD mode is ended by switching to measuring mode (hold **meas** key depressed). The display reads “Good Bye”, after that, the HOLD mode is exited.

When the calibration mode is exited, a confirmation prompt ensures that the installation is ready for operation (e.g.: sensor reinstalled, located in process).

Alarm

External activation of HOLD

The HOLD mode can be activated from outside by sending a signal to the HOLD input (e.g. from the process control system).

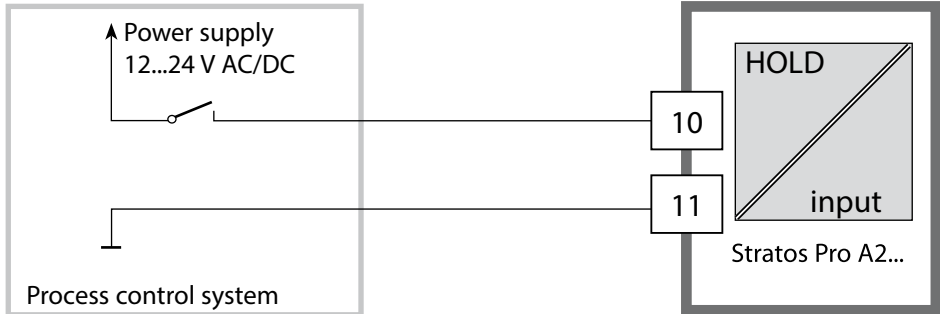

HOLD inactive	0...2 V AC/DC
HOLD active	10...30 V AC/DC

Manual activation of HOLD

The HOLD mode can be activated manually from the HOLD menu. This allows checking or replacing a sensor, for example, without provoking unintended reactions at the outputs.

Press **meas** key to return to selection menu.

Alarm

When an error has occurred, **Err xx** is displayed immediately.

Only after expiry of a user-defined delay time will the alarm be registered and entered in the logbook.

During an alarm the display blinks, the display backlighting turns **red**.

Error messages can also be signaled by a 22 mA output current (see Configuration).

2 sec after the failure event is corrected, the alarm status will be deleted.

Alarm and HOLD Messages

Message	Released by	Cause
Alarm	Sensocheck	Polarization / Cable
(22 mA)	Error Messages	Flow (CONTROL input)
HOLD	HOLD	HOLD via menu or input
(Last/Fix)	CONF	Configuration
	CAL	Calibration
	SERVICE	Service

Generating a message via the CONTROL input (min. flow / max. flow)

The CONTROL input can be used for parameter set selection or for flow measurement (pulse principle), depending on its assignment in the “Configuration” menu.

When preset to flow measurement


CONF/CNTR_IN/CONTROL = FLOW

an alarm can be generated when the measured flow exceeds a specified range:

CONF/ALA/FLOW CNTR = ON

CONF/ALA/FLOW min (specify value, default: 5 liters/h)

CONF/ALA/FLOW max (specify value, default: 25 liters/h)

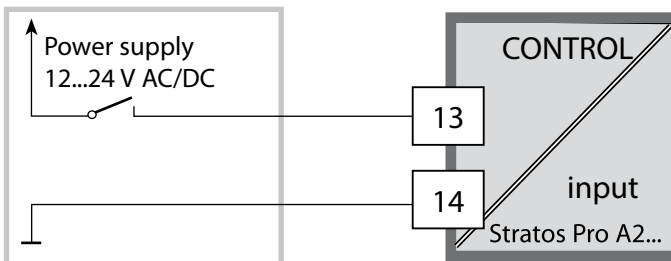

Configuration

Menu Structure of Configuration

The device provides 2 parameter sets "A" and "B". By switching between the parameter sets you can adapt the device to different measurement situations, for example.

Parameter set "B" only permits setting of process-related parameters.

The configuration steps are assigned to different menu groups.

With the left/right arrow keys you can jump between the individual menu groups.

Each menu group contains menu items for setting the parameters.

Pressing **enter** opens a menu item. Use the arrow keys to edit a value.

Press **enter** to confirm/save the settings.

Return to measurement: Hold **meas** key depressed (> 2 s).

Select menu group	Menu group	Code	Display	Select menu item
	Sensor selection	SNS:		 enter enter enter enter
		Menu item 1		
		:		
		Menu item ...		
▶	Current output 1	OT1:		
▶	Current output 2	OT2:		
▶	Compensation	COR:		
▶	Control input (parameter set or flow measurement)	IN:		
▶	Alarm mode	ALA:		◀
▶	Setting the clock	CLK:		◀
▶	Tag number	TAG:		◀


Parameter set A/B: configurable menu groups

The device provides 2 parameter sets "A" and "B". By switching between the parameter sets you can adapt the device to different measurement situations, for example. Parameter set "B" only permits setting of process-related parameters.

Menu group	Parameter set A	Parameter set B
SENSOR	Sensor selection	---
OUT1	Current output 1	Current output 1
OUT2	Current output 2	Current output 2
CORRECTION	Compensation	Compensation
CNTR_IN	Control input	---
ALARM	Alarm mode	Alarm mode
PARSET	Parameter set selection	---
CLOCK	Setting the clock	---
TAG	TAG of measuring point	
GROUP	GROUP of measuring points	

External switchover of parameter sets A/B

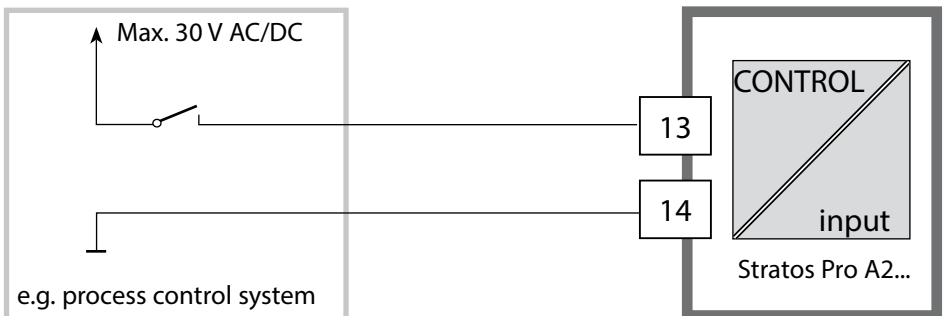

You can switch between parameter sets A and B by applying a signal to the CONTROL input (parameter setting: CNTR-IN – PARSET).



Parameter set A active	0...2 V AC/DC
Parameter set B active	10...30 V AC/DC

Configuration

Manual Switchover of Parameter Sets A/B

Display	Action	Remark
	To switch between parameter sets: Press meas .	Manual selection of parameter sets must have been preset in CONFIG mode. Default setting is a fixed parameter set A. Wrong settings change the measurement properties!
	PARSET blinks in the lower line. Select parameter set using ◀ and ▶ keys	
	Select PARSET A / PARSET B	
	Press enter to confirm. Cancel by pressing meas	

Configuration		Choices	Default
Sensor (SENSOR)			
SNS:	(Select text line)	MEMOSENS STANDARD* TRACES* (TAN)	MEMOSENS
<p>*) These sensors appear in the menu selection but can only be used with a measuring module installed. Stratos Pro A2... MSOXY is intended for connecting a Memosens sensor via RS-485 interface. It does not provide a measuring module. For information on retrofitting and the respective costs, please contact the manufacturer (see back of this manual).</p>			
MEAS MODE		dO % dO mg/l dO ppm GAS %	dO %
TEMP UNIT		°C / °F	°C
CAL MODE		CAL AIR CAL WTR	CAL AIR
CAL TIMER		ON/OFF	OFF
ON	CAL-CYCLE	0...9999 h	0168 h
Memosens	CIP COUNT		ON/OFF
	ON	CIP CYCLES	0...9999 CYC
	SIP COUNT		ON/OFF
	ON	SIP CYCLES	0...9999 CYC
	AUTOCLAVE		ON / OFF
	CHECK TAG/ GROUP		ON / OFF

Configuration

Configuration		Choices	Default
Output 1 (OUT1, no trace measurement)			
OT1:	CHANNEL	OXY/TMP	OXY
	OXY dO %	BEGIN 4mA	000.0...600.0 %
		END 20 mA	0.000...600.0 %
	OXY dO mg/l	BEGIN 4mA	00.00...99.99 mg/l
		END 20 mA	00.00...99.99 mg/l
	OXY dO ppm	BEGIN 4mA	00.00...99.99 ppm
		END 20 mA	00.00...99.99 ppm
	OXY GAS %	BEGIN 4mA	00.00...99.99 %
		END 20 mA	00.00...99.99 %
	TMP °C	BEGIN 4mA	-20...150 °C
		END 20 mA	-20...150 °C
	TMP °F	BEGIN 4mA	-4...302 °F
		END 20 mA	-4...302 °F
	FILTERTIME	0...120 SEC	0000 SEC
	22mA FAIL	ON/OFF	OFF
	22mA FACE	ON/OFF	OFF
	HOLD MODE	LAST/FIX	LAST
	FIX	HOLD-FIX	4...22 mA
			021.0 mA

Configuration		Choices	Default	
Output 1 (OUT1)				
Trace measurement, sensor type 01, TAN required				
These values are specified by the Memosens trace sensor.				
OT1:	CHANNEL		OXY/TMP	OXY
	OXY dO %	BEGIN 4mA (0 mA)	000.0...150.0 %	000.0 %
		END 20 mA	000.0...150.0 %	150.0 %
	OXY dO mg/l	BEGIN 4mA (0 mA)	0000 µg/l...20.00 mg/l	
		END 20 mA	0000 µg/l...20.00 mg/l	
	OXY dO ppm	BEGIN 4mA (0 mA)	0000 ppb...20.00 ppm	
		END 20 mA	0000 ppb...20.00 ppm	
	OXY GAS %	BEGIN 4mA (0 mA)	0000 ppm... 50.00 %	
		END 20 mA	0000 ppm... 50.00 %	
	TMP °C	BEGIN 4mA (0 mA)	-20...150 °C	
		END 20 mA	-20...150 °C	
	TMP °F	BEGIN 4mA (0 mA)	-4...302 °F	
		END 20 mA	-4...302 °F	
	FILTERTIME		0...120 SEC	0000 SEC
	22mA FAIL		ON/OFF	OFF
	22mA FACE		ON/OFF	OFF
HOLD MODE		LAST/FIX	LAST	
FIX	HOLD-FIX	(0) 4...22 mA	021.0 mA	

Configuration

Configuration		Choices	Default	
Output 1 (OUT1)				
Trace measurement, sensor type 001, TAN required				
OT1:	CHANNEL		OXY/TMP	OXY
	OXY dO %	BEGIN 4mA	000.0...150.0 %	000.0 %
		END 20 mA	000.0...150.0 %	150.0 %
	OXY dO mg/l	BEGIN 4mA	000.0 µg/l... 20.00 mg/l	
		END 20 mA	000.0 µg/l... 20.00 mg/l	
	OXY dO ppm	BEGIN 4mA	000.0 ppb... 20.00 ppm	
		END 20 mA	000.0 ppb... 20.00 ppm	
	OXY GAS %	BEGIN 4mA	0000 ppb...50 %	
		END 20 mA	0000 ppb...50 %	
	TMP °C	BEGIN 4mA	-20...150 °C	
		END 20 mA	-20...150 °C	
	TMP °F	BEGIN 4mA	-4...302 °F	
		END 20 mA	-4...302 °F	
	FILTRTIME		0...120 SEC	0000 SEC
	22mA FAIL		ON/OFF	OFF
	22mA FACE		ON/OFF	OFF
HOLD MODE		LAST/FIX	LAST	
FIX	HOLD-FIX	4...22 mA	021.0 mA	

Configuration		Choices	Default		
Output 2 (OUT2)					
OT2:	CHANNEL	OXY/TMP	TMP		
	... other steps like output 1				
Salinity or pressure compensation (CORRECTION)					
COR:	SALINITY		00.00...45.00 ppt	00.00 ppt	
	PRESSURE UNIT		BAR/KPA/PSI	BAR	
	PRESSURE		MAN/EXT *)		
	MAN	BAR	0.000...9.999 BAR	1.013 BAR	
		KPA	000.0...999.9 KPA		
		PSI	000.0...145.0 PSI		
	EXT	I-Input		OFF/4(0)...20 mA	4...20 mA
		BAR	BEGIN 4mA (0 mA)	0.000...9.999 BAR	0.000 BAR
			END 20 mA	0.000...9.999 BAR	9.999 BAR
		KPA	BEGIN 4mA (0 mA)	000.0...999.9 KPA	
			END 20 mA	000.0...999.9 KPA	
		PSI	BEGIN 4mA (0 mA)	000.0...145.0 PSI	
END 20 mA	000.0...145.0 PSI				
Control input (CNTR_IN)					
IN:	CONTROL		PARSET, FLOW	PARSET	
	FLOW	FLOW ADJUST	12000 pulses/liter	0 ... 20000 pulses/liter	
Alarm (ALARM)					
ALA:	DELAYTIME		0...600 SEC	0010 SEC	
	SENSOCHECK		ON/OFF	OFF	
	FLOW CNTR **)		ON/OFF	OFF	
	ON	FLOW MIN **)	005.0 L/h	0 ... 99.9 L/h	
		FLOW MAX**)	025.0 L/h	0 ... 99.9 L/h	

*) only displayed if enabled

**) Hysteresis fixed at 5% of threshold value

Configuration

Configuration		Choices	Default
Parameter set (PARSET)			
PAR:	Select fixed parameter set (A) or switch between A/B via control input or manually in measuring mode	PARSET FIX A/ CNTR INPUT / MANUAL	PARSET FIX A (fixed parameter set A)
Real-time clock (CLOCK)			
CLK:	FORMAT	24 h / 12 h	
	24 h	TIME hh/mm	00..23:00...59
	12 h	TIME hh/mm	00...11 AM/PM: 00...59
	DAY/MONTH		01...31/01...12
	YEAR		2000...2099
Measuring points (TAG / GROUP)			
TAG:	(Input in text line)	A...Z, 0...9, - + < > ? / @	
GROUP:	(Input in text line)	0000...9999	0000

Two complete parameter sets are stored in the EEPROM.
As delivered, the two sets are identical but can be edited.

Note:

Fill in your configuration data on the following pages or use them as original for copy.

Parameter Sets (Original for Copy)

Parameter	Parameter set A	Parameter set B
SNS: Sensor type		--- *)
SNS: Measuring mode		--- *)
SNS: Temperature unit		--- *)
SNS: Calibration mode		--- *)
SNS: Calibration timer		--- *)
SNS: Calibration cycle		--- *)
SNS: CIP counter		--- *)
SNS: SIP counter		--- *)
SNS: Autoclaving counter		--- *)
SNS: CHECK TAG		--- *)
SNS: CHECK GROUP		--- *)
OT1: Process variable		
OT1: Current start		
OT1: Current end		
OT1: Filter time		
OT1: FAIL 22 mA (error messages)		
OT1: FACE 22 mA (Sensoface messages)		
OT1: HOLD mode		
OT1: HOLD FIX current		
OT2: Process variable		
OT2: Current start		
OT2: Current end		
OT2: Filter time		
OT2: FAIL 22 mA (error messages)		
OT2: FACE 22 mA (Sensoface messages)		
OT2: HOLD mode		
OT2: HOLD FIX current		

(Original for Copy) Parameter Sets


Parameter	Parameter set A	Parameter set B
COR: Salinity (ppt)		
COR: Pressure unit (BAR, KPA, PSI)		
COR: Pressure (MAN/EXT)		
COR: Ext. current input (Option)		
IN: Parameter set A/B or flow		
IN: (Flow meter) Adjusting pulses/liter		
ALA: Delay		
ALA: Sensocheck on/off		
ALA: Flow control FLOW CNTR on/off		
ALA: Minimum flow (hysteresis fixed at 5 %)		
ALA: Maximum flow (hysteresis fixed at 5 %)		
PAR: Parameter set selection		--- *)
CLK: Time format		--- *)
CLK: Time hh/mm		--- *)
CLK: Day/month		--- *)
CLK: Year		--- *)
TAG: Measuring point (tag number)		
GROUP: Group of measur- ing points		

*) These parameters cannot be adjusted in parameter set B, the values are the same as in parameter set A.

Configuration



Sensor

Select: Sensor type, measuring mode

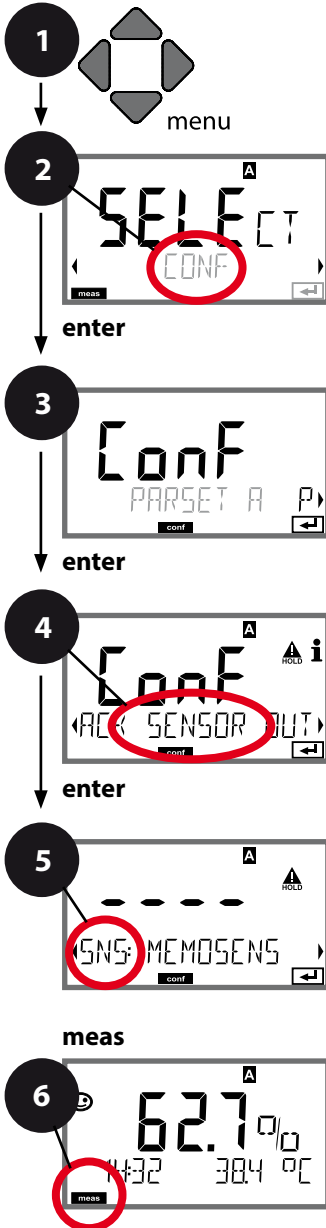

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶, press **enter**.
- 4) Select **SENSOR** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "SNS:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.


Select sensor type	enter
Select measuring mode	enter
Temperature unit	
Calibration medium water/air	
Calibration timer	
CIP/SIP cycles	
Autoclaving counter	
CHECK TAG	
CHECK GROUP	

Menu item	Action	Choices
Select sensor type 	Select sensor type using ▲ ▼ keys. Press enter to confirm.	MEMOSENS STANDARD TRACES (with TAN)
Select measuring mode 	Select measuring mode using ▲ ▼ keys. DO: Measurement in liquids GAS: Measurement in gases Press enter to confirm.	dO % , dO mg/l dO ppm GAS %

Configuration





Sensor

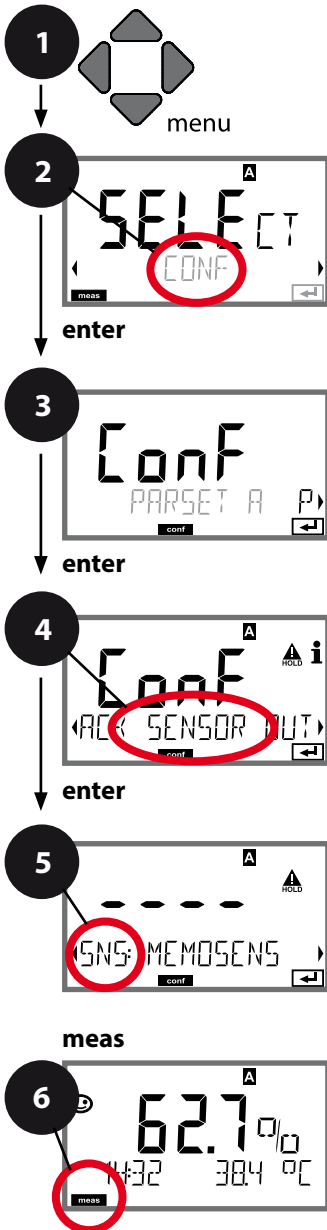Select: Temperature unit, medium: water/air, calibration timer



- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶, press **enter**.
- 4) Select **SENSOR** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "SNS:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Select sensor type	5	enter
Select measuring mode		enter
Temperature unit		enter
Calibration medium water/air		
Calibration timer		
CIP/SIP cycles		
Autoclaving counter		
CHECK TAG		
CHECK GROUP		

Menu item	Action	Choices
Temperature unit 	Select temperature unit using ▲ ▼ keys. Press enter to confirm.	°C °F
Medium: air/water 	Select calibration medium using ▲ ▼ keys. AIR: Air as cal medium WTR: Air-saturated water as cal medium Press enter to confirm.	CAL_AIR CAL_WTR
Calibration timer 	Select/deselect calibration timer using ▲ ▼ keys. Press enter to confirm.	OFF ON
(ON: Calibration cycle) 	Enter calibration cycle in hours using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	0...9999 h 0168 h

Note for the calibration timer:


When Sensocheck has been activated in the Configuration – Alarm menu, the expiration of the calibration interval is indicated by Sensoface (beaker icon and smiley).

The calibration timer settings apply to both parameter sets A and B. The time remaining until the next due calibration can be seen in the diagnostics menu (see “Diagnostics”).

Configuration




Sensor

Adjust: CIP cleaning cycles, SIP sterilization cycles

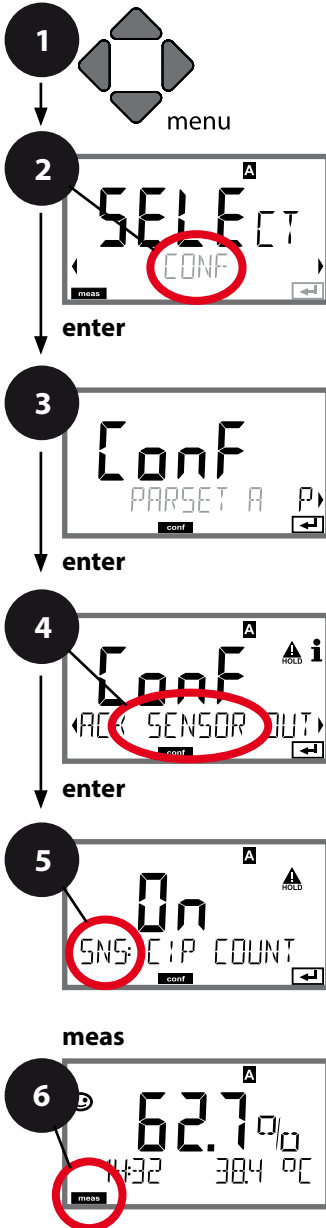

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶, press **enter**.
- 4) Select **SENSOR** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "SNS:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Select sensor type	5	enter
Select measuring mode		enter
Temperature unit		enter
Medium: water/air		
Calibration timer		
CIP cleaning cycle counter		
CIP cleaning cycles		
SIP sterilization cycle counter		
SIP sterilization cycles		
Autoclaving counter		
CHECK TAG		
CHECK GROUP		

Menu item	Action	Choices
CIP counter 	Set CIP counter using ▲ ▼ keys: OFF: No counter ON: Fixed cleaning cycle (adjust in the next step) Press enter to confirm.	OFF/ON
CIP cycles 	Only with CIP COUNT ON: Enter max. number of cleaning cycles using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	0...9999 CYC (0000 CYC)
SIP counter 	Set SIP counter using ▲ ▼ keys: OFF: No counter ON: Max. sterilization cycles (adjust as for CIP counter) Press enter to confirm.	OFF/ON

The cleaning and sterilization cycles are logged to measure the load on the sensor.

Suitable for biochemical applications (process temp approx. 0 ... +50 °C / +32 ... +122 °F, CIP temp > +55 °C / +131 °F, SIP temp > +115 °C / +239 °F).

Note:






A CIP or SIP cycle is only entered into the logbook 2 hours after the start to ensure that the cycle is complete.

With Memosens, an entry is also made in the sensor.


Configuration

Sensor

Adjust: Autoclaving counter

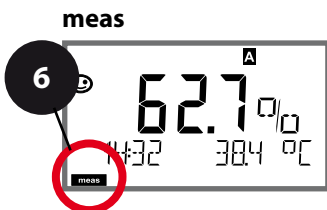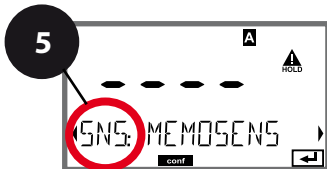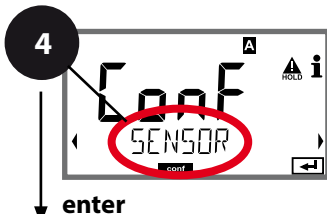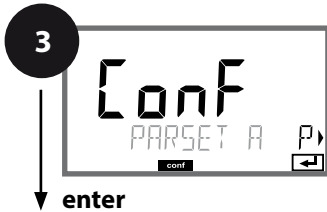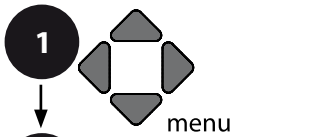

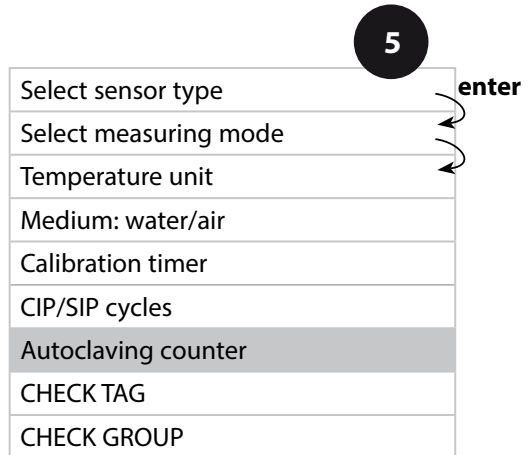

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **SENSOR** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "SNS:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.




Autoclaving Counter

After reaching a specified limit value the autoclaving counter generates a Sensoface message. As soon as the counter has reached the specified value, Sensoface is getting "sad". Pressing the info key shows the text "AUTOCLAVE CYCLES OVERRUN" which reminds you that the maximum number of autoclaving cycles has been reached. After each autoclaving process, you must manually increment the autoclaving counter in the SENSOR service menu on the transmitter. The transmitter displays "INCREMENT AUTOCLAVE CYCLE" as confirmation. You can configure the current outputs so that a Sensoface message generates a 22-mA error signal, see page 59.

Menu item	Action	Choices
Autoclaving counter 	Select using ▲ ▼ keys: ON: The cycles are specified manually (0 ... 9999) Press enter to confirm.	OFF/ON
Incrementing the autoclaving counter (SERVICE menu)	After having completed an autoclaving process, open the SERVICE menu SENSOR / AUTOCLAVE to increment the autoclaving count. To do so, select " YES " and confirm by pressing enter .	NO / YES
		



Configuration

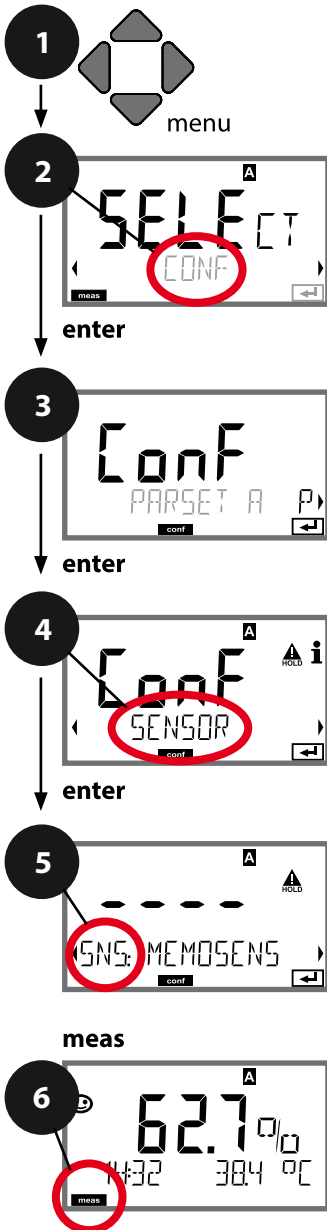Memosens Sensor Sensor Verification (TAG, GROUP)



- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **SENSOR** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "SNS:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Select sensor type	5	enter
Select measuring mode		enter
Temperature unit		enter
Medium: water/air		
Calibration timer		
CIP/SIP cycles		
Autoclaving counter		
CHECK TAG		
CHECK GROUP		

Menu item	Action	Choices
<p>TAG</p> 	<p>Select ON or OFF using ▲ ▼ keys. Press enter to confirm.</p> <p>When switched on, the entry for "TAG" in the Memosens sensor is compared to the entry in the analyzer. If the entries differ, a message will be generated.</p>	<p>ON/OFF</p>
<p>GROUP</p> 	<p>Select ON or OFF using ▲ ▼ keys. Press enter to confirm.</p> <p>Function as described above</p>	<p>ON/OFF</p>

Sensor Verification (TAG, GROUP)


When Memosens sensors are calibrated in the lab, it is often useful and sometimes even mandatory that these sensors will be operated again at the same measuring points or at a defined group of measuring points. To ensure this, you can save the respective measuring point (TAG) or group of measuring points (GROUP) in the sensor. TAG and GROUP can be specified by the calibration tool or automatically entered by the transmitter. When connecting an MS sensor to the transmitter, it can be checked if the sensor contains the correct TAG or belongs to the correct GROUP. If not, a message will be generated, Sensoface gets "sad", and the display backlighting turns purple. The "sad" Sensoface icon can also be signaled by a 22 mA error current. Sensor verification can be switched on in the Configuration in two steps as TAG and GROUP if required.

When no measuring point or group of measuring points is saved in the sensor, e.g., when using a new sensor, Stratos enters its own TAG and GROUP. When sensor verification is switched off, Stratos always enters its own measuring point and group. A possibly existing TAG/GROUP will be overwritten.

Configuration



Current Output 1

Output current range, current start, current end

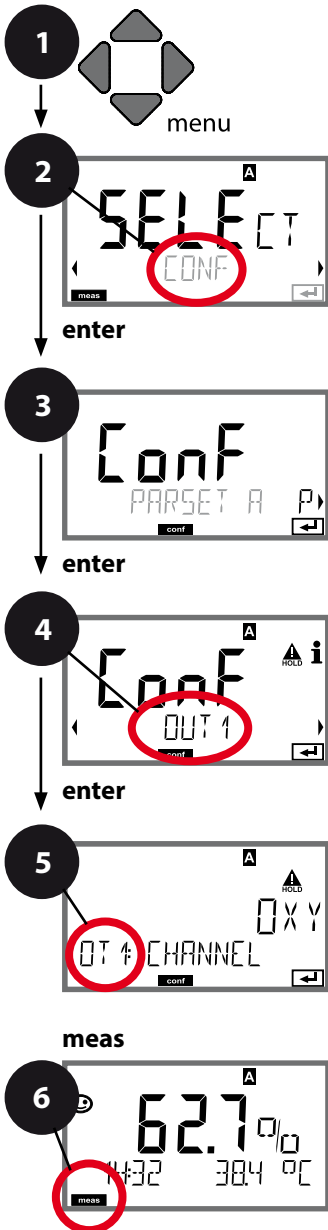

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **OUT1** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "OT1:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Process variable	enter
Current start	enter
Current end	enter
Time averaging filter	
Output current for error message	
Output current for Sensoface	
Output current during HOLD	
Output current for HOLD FIX	

Menu item	Action	Choices
Process variable 	Select using \blacktriangle \blacktriangledown keys: OXY: Oxy value TMP: Temperature Press enter to confirm.	OXY/TMP
Current start, current end 	Modify digit using \blacktriangle \blacktriangledown keys, select next digit using \blacktriangleleft \blacktriangleright keys. Press enter to confirm.	000.0...0600% (OXY) 0.000...0150% (OXY, Traces option) -20...150 °C / -4...302 °F (TMP)


For **process variables comprising several decades**, decimal point and dimension can be shifted using the \blacktriangleleft \blacktriangleright cursor keys.

Then, the desired number is entered using (up / down) and \blacktriangleleft \blacktriangleright .

For measurement in gases (GAS), this method is used to switch between ppm and % for volume concentration (10000 ppm = 1 %).


Assignment of measured values: Current start and current end

Example 1: Range 0...100%

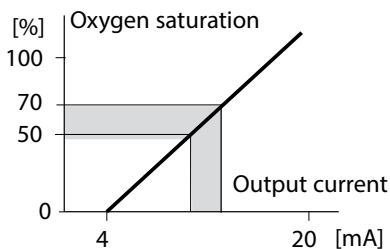

Example 2: Range 50...70%





Advantage: Higher resolution in range of interest

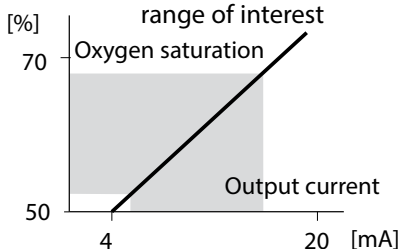

Configuration

Current Output 1


Adjust time interval of output filter

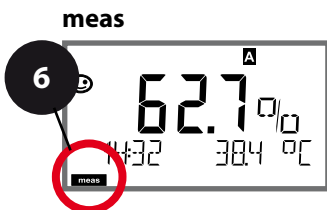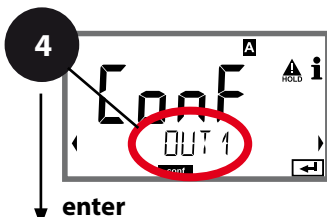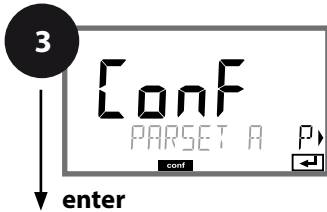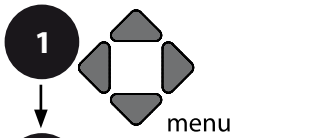

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **OUT1** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "OT1:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

5

Process variable	enter
Current start	enter
Current end	enter
Time averaging filter	
Output current for error message	
Output current for Sensoface	
Output current during HOLD	
Output current for HOLD FIX	

Menu item	Action	Choices
Time averaging filter	Enter value using ▲ ▼ ◀ ▶ keys.	0...120 SEC (0000 SEC)
		
Press enter to confirm.		


Time averaging filter

To smoothen the current output, a low-pass filter with adjustable filter time constant can be switched on. When there is a jump at the input (100 %), the output level is at 63 % after the time interval has been reached. The time interval can be set from 0 to 120 sec. If the time interval is set to 0 sec, the current output directly follows the input.

Please note:

The filter only acts on the current output, not on the display or the limit value!





During HOLD the filter is not applied. This prevents a jump at the output.

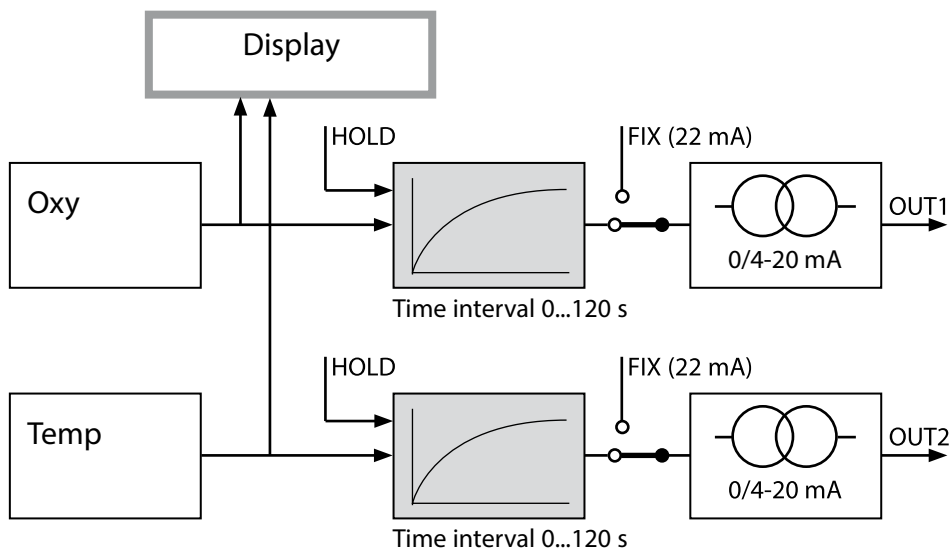

Configuration

Current Output 1



Output current for error message or Sensoface alert

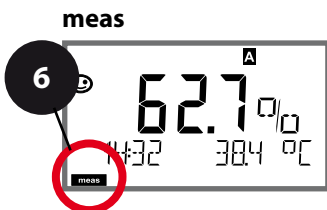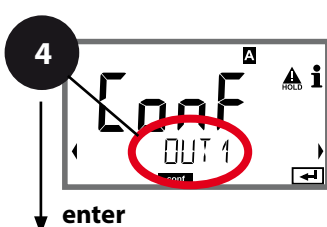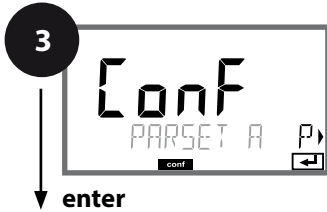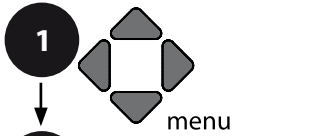


- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **OUT1** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "OT1:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

5

Process variable	enter
Current start	enter
Current end	
Time averaging filter	
Output current for error message	
Output current for Sensoface	
Output current during HOLD	
Output current for HOLD FIX	





Menu item	Action	Choices
Output current for error message (FAIL) 	In the case of an error (FAIL), the current output is set to 22 mA. Select ON or OFF using ▲ ▼ keys. Press enter to confirm.	ON/OFF
Output current for Sensoface (FACE) 	In the case of a Sensoface alert (FACE), the current output is set to 22 mA. Select ON or OFF using ▲ ▼ keys. Press enter to confirm.	ON/OFF

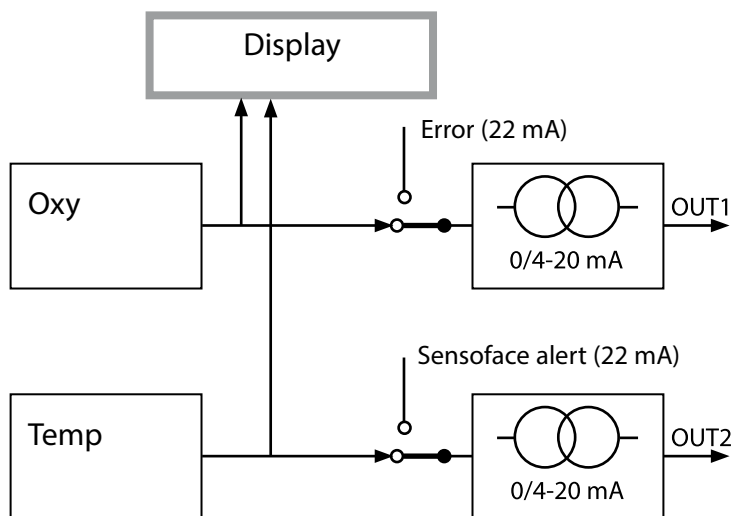

Error messages and Sensoface alerts can be set separately for both current outputs. This allows, for example, signaling error messages only over current output 1 and Sensoface alerts only over current output 2.

Configuration

Current Output 1 Output current during HOLD

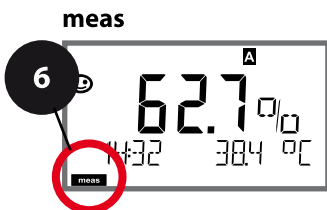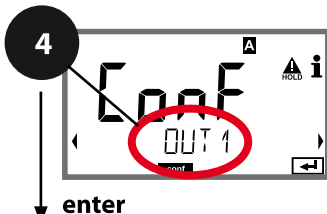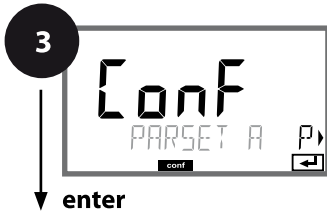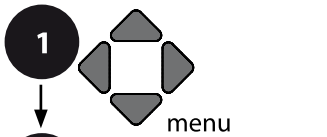

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **OUT1** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "OT1:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.


5

Process variable	enter
Current start	enter
Current end	
Time averaging filter	
Output current for error message	
Output current for Sensoface	
Output current during HOLD	
Output current for HOLD FIX	

Menu item	Action	Choices
Output current during HOLD	LAST: During HOLD the last measured value is maintained at the output. FIX: During HOLD a value (to be entered) is maintained at the output. Select using ▲ ▼ Press enter to confirm.	LAST/FIX
Output current for HOLD FIX	Only with FIX selected: Enter current which is to flow at the output during HOLD Enter value using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	00.40...22.00 mA 21.00 mA

Output signal during HOLD:


Output current [mA]

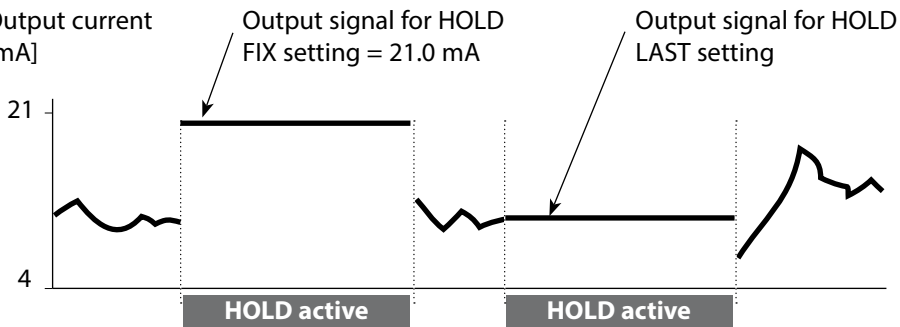

Configuration


Current Output 2

Process variable. Current start. Current end ...

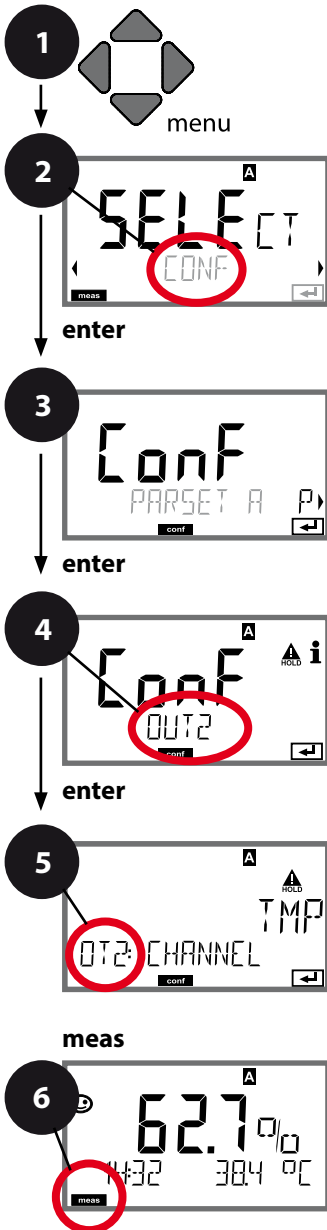

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **OUT2** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "OT2:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Process variable
Current start
Current end
Time averaging filter
Output current for error message
Output current for Sensoface
Output current during HOLD
Output current for HOLD FIX





Menu item	Action	Choices
Process variable 	Select using ▲ ▼ keys: OXY: Oxy value TMP: Temperature Press enter to confirm.	OXY/TMP
<ul style="list-style-type: none"> • • • 		

All the following adjustments are made as for current output 1 (see there)!


Configuration






Correction

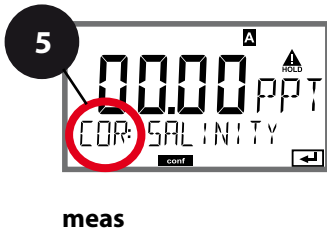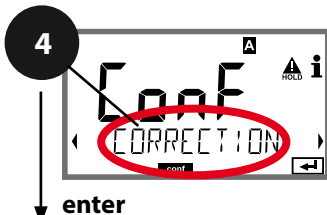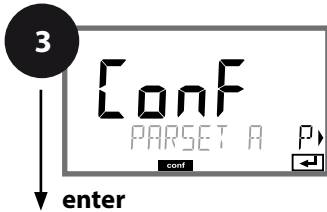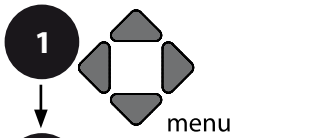Salinity correction. Pressure correction. Current input

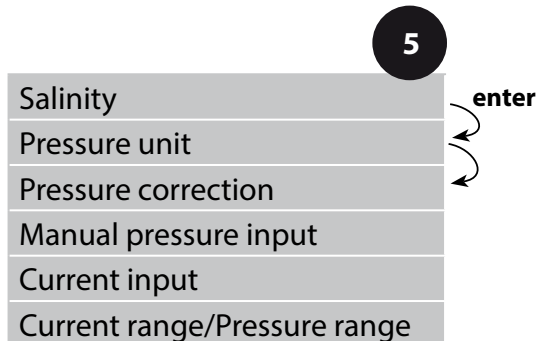

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **CORRECTION** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "COR:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.







Menu item	Action	Choices
Enter salinity 	Enter salinity of the process medium. Enter value using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	00.00...45.00 ppt
Enter pressure unit 	Select desired pressure unit using ▲ ▼ keys. Press enter to confirm.	Bar /kPa/PSI
Enter pressure correction 	Select desired procedure for pressure correction using ▲ ▼ keys: MAN: Manual specification EXT: External pressure correction via current input Press enter to confirm.	MAN / EXT
(Manual pressure input) 	Enter value using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	Input range: 0.000...9.999 BAR / 000.0...999.9 KPA / 000.0...145.0 PSI 1.013 BAR
Current input/ Pressure range 	With external pressure input, select current input 0/4 ... 20 mA and the pressure parameters for current start and end using ▲ ▼ ◀ ▶ keys.	0(4)...20 mA 0.000...9.999 Bar / 000.0...999.9 kPa / 000.0...999.9 PSI


Configuration




CONTROL Input

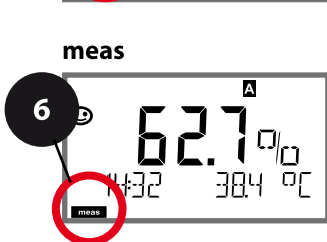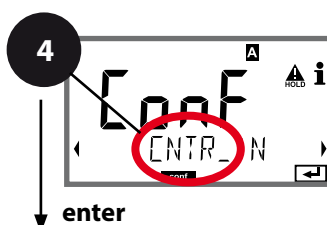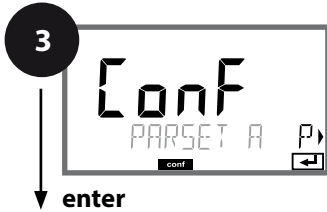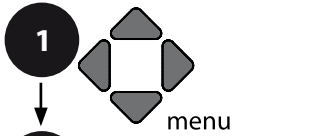Parameter set selection via external signal or flow measurement

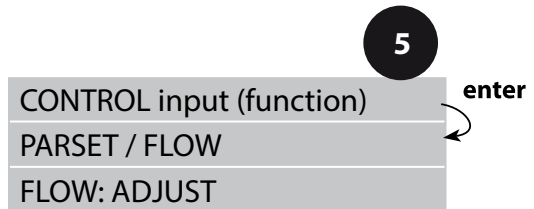

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **CNTR_IN** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "IN:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) using **enter**.
- 6) End: Press **meas** key until the [meas] mode indicator is displayed.



Menu item	Action	Choices
Select function of CONTROL input 	Select using ▲ ▼ keys. Press enter to confirm.	PARSET (selecting parameter set A/B via signal at CONTROL input)
		Flow (for connecting a pulse-output flow meter)
Adjust to flow meter: 	With "Flow" selected, you must adjust the device to the flow meter used. Enter value using arrow keys. Press enter to confirm.	12000 pulses/liter

In the alarm menu you can configure flow monitoring. When you have set CONTROL to FLOW, you can specify 2 additional limit values for maximum and minimum flow.

If the measured value lies outside this range, an alarm message and a 22-mA error signal (if configured) will be generated.

Display

Flow measurement in measuring mode



Display


Flow measurement (sensor monitor)



Configuration



Alarm

Alarm delay. Sensocheck.

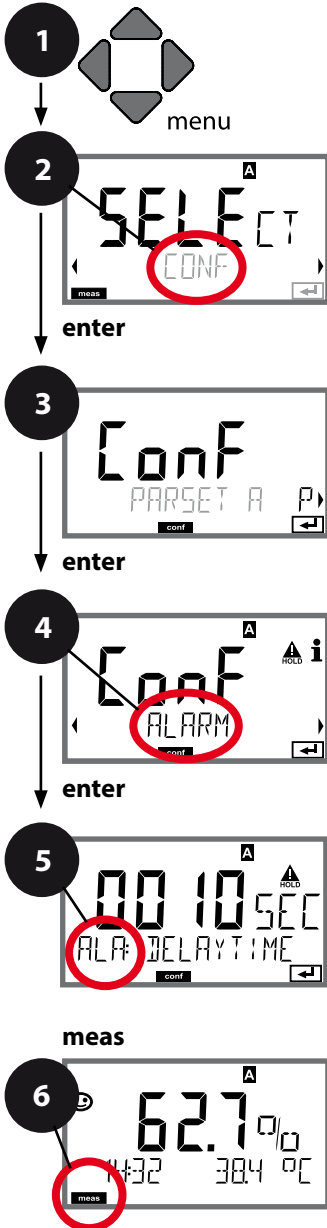

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **ALARM** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "ALA:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

Delay	5	enter
Sensocheck		
Alarm: CONTROL input		
For flow monitoring: Max. flow alarm		
For flow monitoring: Min. flow alarm		

Menu item	Action	Choices
Alarm delay 	Enter alarm delay using ▲ ▼ ◀ ▶ keys. Press enter to confirm.	0...600 SEC (010 SEC)
Sensocheck 	Select Sensocheck (con- tinuous monitoring of sensor membrane and lines). Select ON or OFF using ▲ ▼ keys. Press enter to confirm. (At the same time, Sensoface is activated. With OFF, Sensoface is also switched off.)	ON/OFF




Error messages can be signaled by a 22 mA output current (see Error Messages and Configuration of Output 1/Output 2).

The **alarm delay time** delays the color change of the display backlighting to red and the 22 mA signal (if configured).


Configuration


Alarm Settings

CONTROL input (FLOW MIN, FLOW MAX)

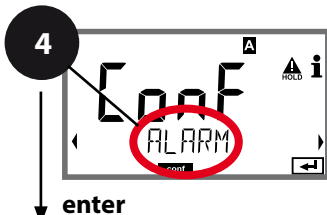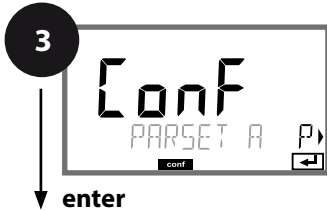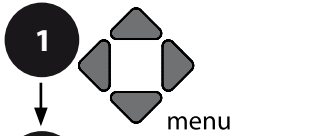


- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶ keys, press **enter**.
- 3) Select parameter set using ◀ ▶ keys, press **enter**.
- 4) Select **ALARM** menu using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "ALA:" code.
Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) using **enter**.
- 6) End: Press **meas** key until the [meas] mode indicator is displayed.

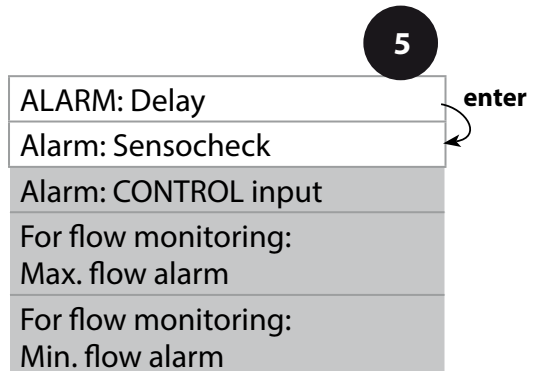


Menu item	Action	Choices
CONTROL input 	The CONTROL input can generate an alarm when assigned to FLOW (flow monitoring) in the CONF menu: FLOW CNTR Flow measurement: allows monitoring the minimum and maximum flow (pulse counter)	ON/OFF (FLOW MIN, FLOW MAX.)
Alarm Minimum flow FLOW MIN	Specify value	Default: 05.00 liters/h
Alarm Maximum flow FLOW MAX	Specify value	Default: 25.00 liters/h

Configuration

Time and Date Measuring Points (TAG/GROUP)

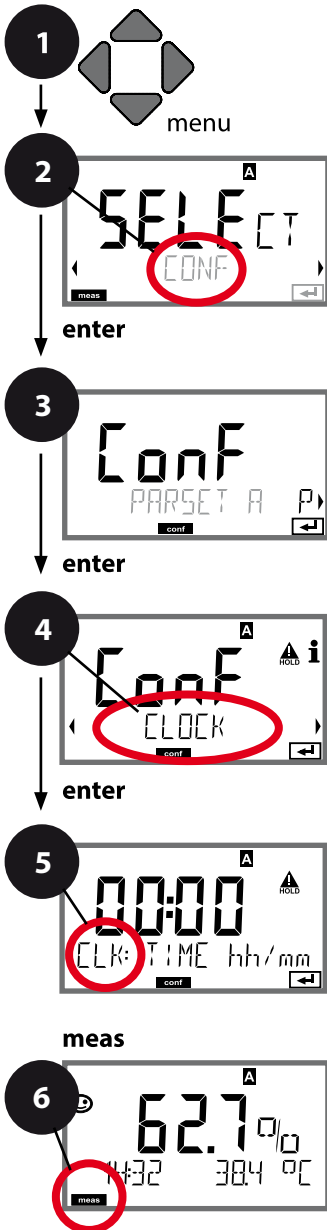

- 1) Press **menu** key.
- 2) Select **CONF** using ◀ ▶, press **enter**.
- 3) Select parameter set A using ◀ ▶ keys, press **enter**.
- 4) Select **CLOCK** or **TAG** using ◀ ▶ keys, press **enter**.
- 5) All items of this menu group are indicated by the "CLK:" or "TAG" code. Press **enter** to select menu, edit using arrow keys (see next page). Confirm (and proceed) by pressing **enter**.
- 6) Exit: Press **meas** key until the [meas] mode indicator is displayed.

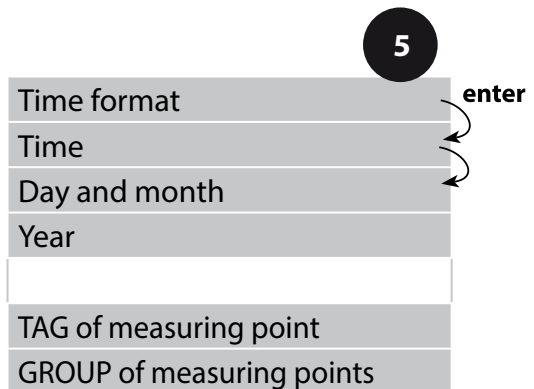

Time and Date

Control of the calibration and cleaning cycles is based on the time and date of the integrated real-time clock.

In measuring mode the time is shown in the lower display. When using digital sensors, the calibration data is written in the sensor head. In addition, the logbook entries (cf Diagnostics) are provided with a time stamp.


Note:

There is no automatic switchover from winter to summer time!
Be sure to manually adjust the time!

Sensor Verification (TAG, GROUP)

When Memosens sensors are calibrated in the lab, it is often useful and sometimes even mandatory that these sensors will be operated again at the same measuring points or at a defined group of measuring points. To ensure this, you can save the respective measuring point (TAG) or group of measuring points (GROUP) in the sensor. TAG and GROUP can be specified by the calibration tool or automatically entered by the transmitter. When connecting an MS sensor to the transmitter, it can be checked if the sensor contains the correct TAG or belongs to the correct GROUP. If not, a message will be generated, Sensoface gets “sad”, and the display backlighting turns purple. The “sad” Sensoface icon can also be signaled by a 22 mA error current. Sensor verification can be switched on in the Configuration in two steps as TAG and GROUP if required.

When no measuring point or group of measuring points is saved in the sensor, e.g., when using a new sensor, Stratos enters its own TAG and GROUP. When sensor verification is switched off, Stratos always enters its own measuring point and group. A possibly existing TAG/GROUP will be overwritten.

Menu item	Action	Choices
Measuring point (TAG) 	In the lower display line you can enter a designation for the measuring point (TAG) and for a group of measuring points (GROUP) if applicable. Up to 32 digits are possible. By pressing meas (repeatedly) in the measuring mode you can view the tag number. Select character using ▲ ▼ keys, select next digit using ◀ ▶ keys. Press enter to confirm.	A...Z, 0...9, - + < > ? / @ The first 10 characters are seen in the display without scrolling.

Digital Sensors

Stratos Pro can be operated with digital sensors. Due to the galvanic isolation of Memosens sensors, earth or ground potentials have no effect here. Therefore, a Solution Ground or measures for equipotential bonding are not required.

Digital sensors can be calibrated and maintained in the lab. This considerably simplifies on-site maintenance.

Memosens Sensors: Calibration and Maintenance in the Lab

The “MemoSuite” software allows calibrating Memosens sensors under reproducible conditions at a PC in the lab. The sensor parameters are registered in a database. Documenting and archiving meet the demands of FDA CFR 21 Part 11. Detailed reports can be output as csv export for Excel.

Settings and specifications

Currently connected sensor:
Sensor type, manufacturer, order code and serial number

Function selection
(The selected function is highlighted.)

Parameters of currently connected sensor

Last calibration
(adjustment)

Measured values	
Oxygen current	-141 nA
Oxygen current (25 °C)	-143 nA
Temperature	24.5 °C
Partial pressure	214.3 hPa
Percent saturation (water)	104.3 %Air
Concentration (water)	7.571 ppm
Oxygen content (gas)	21.19%Vol

Sensor data	
Sensor type:	Oxygen
Manufacturer:	KNICK
Order code:	SE 715/1-MS
Serial number:	1029852

Adjustment data	
Date:	06/29/2011 11:22:56
Slope:	-137 nA
Zero point:	0.00 nA

Measured values

Oxygen current	-141 nA
Oxygen current (25 °C)	-143 nA

Display size of measured values:
When the cursor moves over a measured value, it changes to a magnifying glass, allowing to magnify the measured-value display at a mouse click.



Calibration history of several sensors




History: Load diagrams of the sensors

Memosens Sensors: Configuring the Device

The sensor type is selected during **Configuration**.

The device only switches to measuring mode when the connected sensor corresponds to the type configured (Sensoface is friendly):





Otherwise, an error message is released. The **info** icon is displayed. You can display the error text in the bottom line using the ◀ ▶ keys.

The comprehensive display options of the software allow drawing conclusions on the aging behavior of the sensors at one glance and making a reliable forecast for predictive maintenance.

The software is available as “Basic” (calibration function) or “Advanced” (with sensor database) version:
www.knick.de



Digital Sensors

Connecting a Digital Sensor

Step	Action/Display	Remark
Connect sensor		Before a digital sensor is connected, the error message "No sensor" is displayed.
Wait until the sensor data are displayed.		The hourglass in the display blinks.
Check sensor data	 <p>View sensor information using ◀ ▶ keys, press enter to confirm.</p>	Display color changes to green . Sensoface is friendly when the sensor data are okay.
Go to measuring mode	Press meas , info or enter	After 60 sec the device automatically returns to measuring mode (time-out).

Replacing a Sensor

A sensor should only be replaced during HOLD mode to prevent unintended reactions of the outputs or contacts. When you first want to calibrate the new sensor, it can also be replaced in calibration mode.

Step	Action/Display	Remark
Select HOLD mode	Press menu key to call the selection menu, select HOLD using the ◀ ▶ keys, press enter to confirm.	Now the device is in HOLD mode. The HOLD mode can also be activated externally via the HOLD input. During HOLD the output current is frozen at its last value or set to a fixed value.
Disconnect old sensor, connect new sensor.		Temporary messages are displayed during the replacement but neither output to the alarm contact nor entered in the logbook.
Wait until the sensor data are displayed.		
Check sensor data	 <p>View sensor information using ◀ ▶ keys, press enter to confirm.</p>	You can view the sensor manufacturer and type, serial number, and last calibration date.
Check measured values, then exit HOLD.	Hit meas key: Return to the selection menu. Hold meas key depressed: Device switches to measuring mode.	The sensor replacement is entered in the extended logbook.

Calibration

Calibration adapts the device to the individual sensor characteristics. It is always recommended to calibrate in air.

Compared to water, air is a calibration medium which is easy to handle, stable, and thus safe. In the most cases, however, the sensor must be removed for a calibration in air.

When dealing with biotechnological processes which require sterile conditions, the sensor cannot be removed for calibration. Here, calibration must be performed with aeration directly in the process medium (e.g. after sterilization).

In the field of biotechnology, for example, often saturation is measured and calibration is performed in the medium for reasons of sterility.

For other applications where concentration is measured (water control etc.), calibration in air has proved to be useful.

Note:

- All calibration procedures must be performed by trained personnel. Incorrectly set parameters may go unnoticed, but change the measuring properties.
- If a 2-point calibration is prescribed, the zero calibration should be performed prior to slope calibration.

Common combination:

process variable / calibration medium

Process variable	Calibration	Default rel. humidity	Default cal pressure
Saturation (%) SAT	Water	+100 %	Process pressure
Concentration (mg/l, ppm) Conc	Air	50 %	1.013 bar

The calibration procedures for these two common applications are described on the following pages. Of course, other combinations of process variable and calibration medium are possible.

Selecting a Calibration Mode

Calibration is used to adapt the device to the individual sensor characteristics, namely zero and slope.

Access to calibration can be protected with a passcode (SERVICE menu).

First, you open the calibration menu and select the calibration mode:

CAL_WTR /	Calibration in air-saturated water / air
CAL_AIR	(as configured)
CAL_ZERO	Zero calibration
P_CAL	Product calibration (calibration with sampling)
CAL-RTD	Temperature probe adjustment







Zero Calibration

Memosens sensors have very low zero currents. Therefore, a zero calibration is only recommended for measurement of oxygen traces.

When a zero calibration is performed, the sensor should remain for at least 10 to 30 minutes in the calibration medium in order to obtain stable, non-drifting values.

During zero calibration, a drift check is not performed. Zero current of a properly functioning sensor is notably less than 0.5 % of air current. The display (bottom: measured value, top: entered value) does not change until an input current is entered for the zero point.

When measuring in an oxygen-free medium, the displayed current can be taken directly.

Display	Action	Remark
	Select calibration, proceed by pressing enter	
	Ready for calibration. Hourglass blinks. Place sensor in oxygen-free medium	Display (3 sec) Now the device is in HOLD mode.
	Upper display line: Zero current. Press enter to save this value or correct using arrow keys and then save by pressing enter . Lower display line: Sensor current measured	
	Display of slope Display of new zero current. End calibration by pressing enter key, place sensor in process	Sensoface display
	The oxygen value is shown in the main display, "enter" blinks. Stop Hold by pressing enter .	New calibration: Select REPEAT, press enter key.
	Quit by pressing enter .	After end of calibration, the outputs remain in HOLD mode for a short time.

Product Calibration

Calibration with sampling

During product calibration the sensor remains in the process.

The measurement process is only interrupted briefly.




Procedure: During sampling the currently measured value is stored in the device.







The device immediately returns to measuring mode.

The cal mode indicator blinks and reminds you that calibration has not been terminated. The reference value is measured on the site, e.g. using a portable DO meter in a bypass.

This value is then entered in the device. The new value for slope or zero is calculated from the stored value and the reference value. From the measured value, the device automatically recognizes whether a new slope or zero must be calculated (above approx. 5 % saturation: slope, below: zero).







If the sample is invalid, you can take over the measured value saved during sampling instead of the reference value. In that case the old calibration values remain stored. Afterwards, you can start a new product calibration. The following describes a product calibration with slope correction – a product calibration with zero correction is performed correspondingly.

Display	Action	Remark
	Select calibration, then product calibration P_CAL. Press enter to proceed.	
	Ready for calibration. Hourglass blinks.	Display (3 sec) Now the device is in HOLD mode.
	Take sample and save value. Press enter to proceed.	Now the sample can be measured. If the value is already available, press info+enter to proceed to step 2.







Display	Action	Remark
	The device returns to measuring mode.	From the blinking CAL mode indicator you see that product calibration has not been terminated.
	Product calibration step 2: When the sample value has been determined, open the product calibration once more	Display (3 sec) Now the device is in HOLD mode.
	The stored value is displayed (blinking) and can be overwritten with the lab value. Press enter to proceed.	
	Display of new slope and zero. Sensoface is active. Press enter to proceed.	Related to 25 °C and 1013 mbar
	Display of new oxy value. Sensoface is active. To end calibration: Select MEAS, then enter	Repeat calibration: Select REPEAT, then enter
	End of calibration	After end of calibration, the outputs remain in HOLD mode for a short time.

Slope Calibration (Medium: Water)






(air-saturated)






Display	Action	Remark
	Select calibration (SLOPE). Immerse sensor in cal medium, start by pressing enter	"CAL WATER" or "CAL AIR" is selected in the configuration.
	Enter cal pressure Press enter to proceed.	Default: 1.000 bar Unit bar/kpa/PSI
	Drift check: Display of: Sensor current (nA) Response time (s) Temperature (°C/°F)	Device goes to HOLD mode. The drift check might take some time.
	Display of calibration data (slope and zero) and Sensoface Press enter to proceed.	Related to 25 °C and 1013 mbar
	Display of selected process value. To end calibration: Select MEAS using ◀ ▶, then enter	To repeat calibration: Select REPEAT using ◀ ▶, then enter
	Place sensor in process. End of calibration	After end of calibration, the outputs remain in HOLD mode for a short time.

Slope Calibration (Medium: Air)

Display	Action	Remark
 The display shows 'CAL' in large letters, 'MEDIUM AIR' below it, and a 'cal' indicator at the bottom left. There is a 'HOLD' icon at the top right.	Select calibration. Place sensor in air, press enter to start. Device goes to HOLD mode.	"CAL WATER" or "CAL AIR" is selected in the configuration.
 The display shows '050.0' in large digits, 'REL HUMIDITY' below it, and a 'cal' indicator at the bottom left. There is a 'HOLD' icon at the top right.	Enter relative humidity using arrow keys Press enter to proceed.	Default for relative humidity in air: rH = 50%
 The display shows '1.000' in large digits, 'BAR' to the right, and 'PRESSURE' below it. There is a 'cal' indicator at the bottom left and a 'HOLD' icon at the top right.	Enter cal pressure using arrow keys Press enter to proceed.	Default: 1.000 bar Unit bar/kpa/PSI
 The display shows '6.13' in large digits, 'nA' to the right. Below it, '120 s' and '27.3 °C' are shown. There is a 'cal' indicator at the bottom left and a 'HOLD' icon at the top right.	Drift check: Display of: Sensor current (nA) Response time (s) Temperature (°C/°F) Press enter to proceed.	The drift check can take some minutes.
 The display shows '-59.3' in large digits, 'nA' to the right. Below it, 'ZERO' and '-003 nA' are shown. There is a 'cal' indicator at the bottom left and a 'HOLD' icon at the top right.	Display of calibration data (slope and zero). Press enter to proceed.	
 The display shows '20.93' in large digits, 'MEAS' below it, and 'REPE' to the right. There is a 'cal' indicator at the bottom left and a 'HOLD' icon at the top right.	Display of selected process variable (here: %vol). Now the device is in HOLD mode: Reinstall the sensor and check whether the message is OK. MEAS ends calibration, REPEAT permits repetition.	After end of calibra- tion, the outputs re- main in HOLD mode for a short time.

Temp Probe Adjustment

Display	Action	Remark
 The display shows 'CAL' in large digits, with 'CAL_RT0' below it. There are navigation arrows on the left and right, and a 'cal' indicator at the bottom left.	Select temp adjustment. Press enter to proceed.	Wrong settings change the measurement properties!
 The display shows 'CAL' in large digits, with 'TEMP ADJUST' below it. There is a 'HOLD' icon at the top right and a 'cal' indicator at the bottom left.	Measure the temperature of the process medium using an external thermometer.	Display (3 sec) Now the device is in HOLD mode.
 The display shows '25.0' in large digits, with '°C' to the right. Below it is 'ADJUST 235°C'. There is a 'HOLD' icon at the top right and a 'cal' indicator at the bottom left.	Enter the measured temperature value. Maximum difference: 10 K. Press enter to proceed.	Display of actual temperature (uncompensated) in the lower display.
 The display shows '25.0' in large digits, with '°C' to the right. Below it is 'MEAS'. There is a smiley face icon at the top left, a 'HOLD' icon at the top right, and a 'cal' indicator at the bottom left.	The corrected temperature value is displayed. Sensoface is active. To end calibration: Select MEAS, then enter To repeat calibration: Select REPEAT, then enter	After end of calibration, the outputs remain in HOLD mode for a short time.
 The display shows '20.93' in large digits, with '°C' to the right. Below it is 'GOOD BYE'. There is a smiley face icon at the top left, a 'HOLD' icon at the top right, and a 'meas' indicator at the bottom left.	After calibration is ended, the device will switch to measuring mode.	

Display	Remark
	<p>From the configuration or calibration menus, you can switch the device to measuring mode by pressing the meas key.</p> <p>(Waiting time for signal stabilization approx. 8 sec.)</p> <p>In the measuring mode the main display shows the configured process variable (Oxy [%] or temperature), the secondary display shows the time and the second configured process variable (Oxy [%] or temperature). The [meas] mode indicator lights and the active parameter set (A/B) is indicated.</p>
<p>or AM/PM and °F:</p>	
	
<p>By pressing the meas key you can step through the following displays. When no key has been pressed for 60 sec, the device returns to the MAIN DISPLAY.</p>	
	<p>1) Selecting the parameter set (if set to "manual" in the configuration). Select the desired parameter set using the ◀ ▶ arrow keys (PARSET A or PARSET B blinks in the lower display line). Press enter to confirm.</p>
	<p>Further displays (each by pressing meas).</p>
	<p>2) Display of tag number ("TAG") 3) Display of time and date</p>

Diagnostics


In the Diagnostics mode you can access the following menus without interrupting the measurement:







CALDATA	viewing the calibration data
SENSOR	viewing the sensor data
SELFTEST	starting a device self-test
LOGBOOK	viewing the logbook entries
MONITOR	displaying currently measured values
VERSION	displaying device type, software version, serial number





Access to diagnostics can be protected with a passcode (SERVICE menu).





Note:

HOLD is not active during Diagnostics mode!






Action	Key	Remark
Activate Diagnostics		Press menu key to call the selection menu. (Display color changes to turquoise.) Select DIAG using ◀ ▶ keys, confirm by pressing enter .
Select diagnostics option		Use ◀ ▶ keys to select from: CALDATA SENSOR SELFTEST LOGBOOK MONITOR VERSION See next pages for further proceeding.
Exit	meas	Exit by pressing meas .

Display	Menu item
	<p>Displaying the calibration data</p> <p>Select CALDATA using ◀ ▶, confirm by pressing enter. Use the ◀ ▶ keys to select the desired parameter from the bottom line of the display: (LAST_CAL ZERO SLOPE NEXT_CAL). The selected parameter is shown in the main display.</p>
	
	<p>Press meas to return to measurement.</p>
	<p>Displaying the sensor data</p> <p>For analog sensors, the type is displayed, for digital sensors, the manufacturer, type, serial number and last calibration date. In each case Sensoface is active.</p>
	<p>Display data using ◀ ▶ keys, press enter or meas to return.</p>
	

Display	Menu item
	<p>Device self-test (To abort, you can press meas.)</p> <ol style="list-style-type: none">1) Display test: Display of all segments with changing background colors (white/green/red). Press enter to proceed.
	<ol style="list-style-type: none">2) RAM test: Hourglass blinks, then display of --PASS-- or --FAIL-- Press enter to proceed.
	<ol style="list-style-type: none">3) EEPROM test: Hourglass blinks, then display of --PASS-- or --FAIL-- Press enter to proceed.
	<ol style="list-style-type: none">4) FLASH test: Hourglass blinks, then display of --PASS-- or --FAIL-- Press enter to proceed.

Display	Menu item
	<p>Displaying the logbook entries Select LOGBOOK using ◀ ▶, press enter to confirm.</p> <p>Using the ▲ ▼ keys, you can scroll backwards and forwards through the logbook (entries -00-...-99-), -00- being the last entry.</p>
	<p>If the display is set to date/time, you can search for a particular date using the ▲ ▼ keys. Press ◀ ▶ to view the corresponding message text.</p>
	<p>If the display is set to the message text, you can search for a particular message using the ▲ ▼ keys. Press ◀ ▶ to display the date and time.</p> <p>Press meas to return to measurement.</p>
	<p>Extended logbook / Audit Trail (via TAN) Using the ▲ ▼ keys, you can scroll backwards and forwards through the extended logbook (entries -000-...-199-), -000- being the last entry.</p> <p>Display: CFR Audit Trail also records function activations (CAL CONFIG SERVICE), some Sensoface messages (cal timer, wear) and opening of the enclosure.</p>

Diagnosics




Display	Menu item
 <p>Display example:</p>  	<p>Displaying the currently measured values (sensor monitor)</p> <p>Select MONITOR using ◀ ▶, press enter to confirm. Use the ◀ ▶ keys to select the desired parameter from the bottom line of the display: I-OXY, I-INPUT, OPERATION TIME, SENSOR WEAR. The selected parameter is shown in the main display. Press meas to return to measurement.</p> <p>Display of directly measured value (for validation, sensor can be immersed in a calibration solution, for example, or the device is checked by using a simulator)</p> <p>Display of sensor operating time</p>
	<p>Display of sensor wear (Memosens only)</p> <p>When Sensocheck is activated, Sensoface will remind you to check the sensor and replace electrolyte and membrane. Info text: "Sensor wear - change membrane and electrolyte". After having carried out the servicing, reset the sensor wear counter in the Service menu.</p>
	<p>Version</p> <p>Display of device type, software/hardware version and serial number for all device components. Use the ▲ ▼ keys to switch between software and hardware version. Press enter to proceed to next device component.</p>





In the Service mode you can access the following menus:




MONITOR	displaying currently measured values
SENSOR	displaying the sensor data, with MEMOSENS also resetting the sensor wear counter after replacement of electrolyte/membrane, incrementing the autoclaving counter
OUT1	testing current output 1
OUT2	testing current output 2
CODES	assigning and editing passcodes
DEFAULT	resetting the device to factory settings
OPTION	enabling options via TAN

Note:

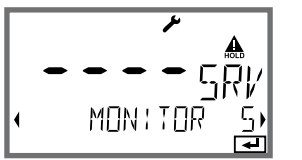































HOLD is active during Service mode!




Action	Key/Display	Remark
Activate Service		Press menu key to call the selection menu. Select SERVICE using ◀ ▶ keys, press enter to confirm.
Passcode		Enter passcode "5555" for service mode using the ▲ ▼ ◀ ▶ keys. Press enter to confirm.
View		In service mode the following icons are displayed: <ul style="list-style-type: none"> • [diag] mode indicator • HOLD triangle • Service (wrench)
Exit	meas	Exit by pressing meas .

Menu item	Remark
	<p>Displaying currently measured values (sensor monitor) with HOLD mode activated: Select MONITOR using ◀ ▶, press enter to confirm. Select variable in the bottom text line using ◀ ▶. The selected parameter is shown in the upper display line.</p> <p>As the device is in HOLD mode, you can perform validations using simulators without influencing the signal outputs.</p> <p>Return to Service menu: Hold meas depressed for longer than 2 sec. Press meas once more to return to measurement.</p>
	<p>Sensor: Resetting the wear counter When you have replaced the electrolyte or the membrane of the OXY sensor, you should reset the wear counter. Default setting is "NO". Select "YES" and press enter to reset the wear counter.</p>
	<p>Incrementing the autoclaving counter After having completed an autoclaving process, you must increment the autoclaving count. To do so, select "YES" and confirm by pressing enter. The device confirms with "INCREMENT AUTOCLAVE CYCLE".</p>
	<p>Specifying the current at outputs 1 and 2: Select OUT1 or OUT2 using the ◀ ▶ keys, press enter to confirm. Enter a valid current value for the respective output using ▲ ▼ ◀ ▶ keys. Press enter to confirm. For checking purposes, the actual output current is shown in the bottom right corner of the display. End by pressing enter or meas.</p>

Menu item	Remark
 <p>The LCD display shows '0000' in large digits. To the right, there is a 'PWR' icon with a triangle above it and 'HOLD' text. Below the digits, 'DIAG' and 'HOLD' are visible as menu options. A right arrow is at the bottom right.</p>	<p>Assigning passcodes: In the "SERVICE - CODES" menu you can assign passcodes to DIAG, HOLD, CAL, CONF and SERVICE modes (Service preset to 5555).</p> <p>When you have lost the Service passcode, you have to request an "Ambulance TAN" from the manufacturer specifying the serial number of your device. To enter the "Ambulance TAN", call the Service function and enter passcode 7321. After correct input of the ambulance TAN the device signals "PASS" for 4 sec and resets the Service passcode to 5555.</p>
 <p>The LCD display shows 'FACTORY SETTING' in large letters. Above it, there are three dashes and a 'NO' with an 'i' icon. A right arrow is at the bottom right.</p>	<p>Reset to factory settings: In the "SERVICE - DEFAULT" menu you can reset the device to factory settings.</p> <p>NOTICE! After a reset to factory setting the device must be reconfigured completely, including the sensor parameters!</p>
 <p>The LCD display shows '0000' in large digits. To the right, there is a 'TAN' icon with a triangle above it. Below the digits, 'OPT: LOGBOOK' is visible. A right arrow is at the bottom right.</p>	<p>Option request: Communicate the serial number and hardware/software version of your device to the manufacturer. These data can be viewed in the Diagnostics/Version menu.</p> <p>The "transaction number" (TAN) you will then receive is only valid for the device with the corresponding serial number.</p> <p>Releasing an option: Options come with a "transaction number" (TAN). To release the option, enter this TAN and confirm by pressing enter.</p>

Operating States


Operating status	OUT 1	OUT 2	Time out
Measuring			-
DIAG			60 s
CAL_ZERO Zero point			No
CAL_SLOPE Slope			No
P_CAL Product calibration S1			No
P_CAL Product calibration S2			No
CAL_RTD Temp adjustment			No
CONF_A ParSet A			20 min
CONF_B ParSet B			20 min
SERVICE MONITOR			20 min
SERVICE OUT 1			20 min
SERVICE OUT 2			20 min
SERVICE CODES			20 min
SERVICE DEFAULT			20 min
SERVICE OPTION			20 min
HOLD input			No

Explanation:  as configured (Last/Fix or Last/Off)
 active  manual

A2...X: Supply Units and Connection

Recommended Power Supply Units:	Order No.:
Repeater power supply, Ex, 90...253 V AC, output 4...20 mA	WG 21 A7
Repeater power supply, Ex, 90...253 V AC, HART, output 4...20 mA	WG 21 A7 Opt. 470
Repeater power supply, Ex, 24 V AC/DC, output 4...20 mA	WG 21 A7 Opt. 336
Repeater power supply, Ex, 24 V AC/DC, HART, output 4...20 mA	WG 21 A7 Opt. 336, 470
Repeater power supply, non-Ex, 24 V DC, output 4...20 mA	IsoAmp PWR B 10116
Repeater power supply, non-Ex, 24 V DC, HART, output 0/4...20 mA / 0...10 V	IsoAmp PWR A 20100

Connection to Supply Units

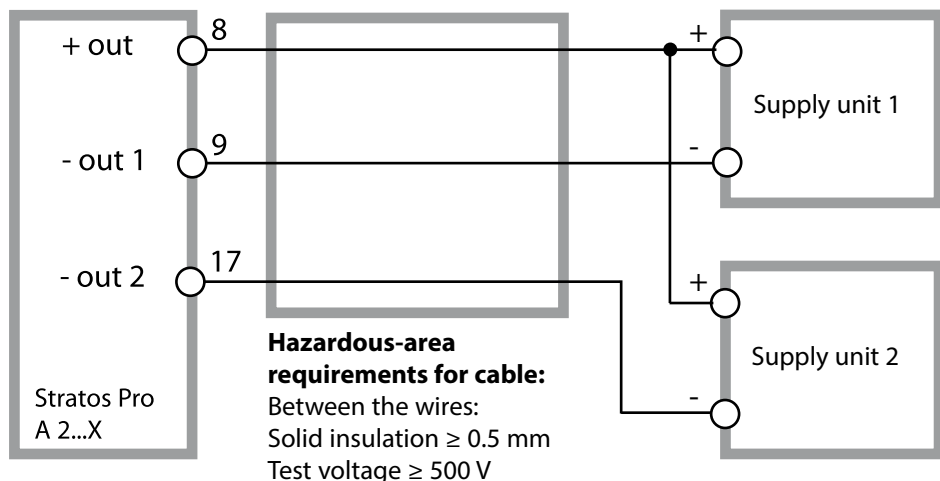

Product Line and Accessories

Order Code Stratos Pro A 2...

Example	A	2	0	1	X	-	MSOXY	-	1	TAN
2-wire / 4-20 mA	A	2								B,C,E
Communication										
Without (HART retrofittable via TAN)			0							A
Version number										
Version				1						
Approvals										
General Safety					N					
ATEX / IECEx Zone 2					B					
ATEX / IECEx / FM / CSA Zone 1 / Cl 1 Div 1					X					
Measuring channel										
Memosens pH / Redox	digital						MSPH			G
Memosens Cond	digital						MSCOND			
Memosens Condi	digital						MSCONDI			
Memosens Oxy	digital						MSOXY			
Dual COND (2x2-electrode sensors, analog)					N		CC			
pH / ORP value (ISM digital per TAN)	Measuring module						PH			F, G
Cond, 2-/4-electrode	Measuring module						COND			
Conductivity, electrodeless	Measuring module						CONDI			
Oxygen (ISM digital and traces per TAN)	Measuring module						OXY			D, F
Options										
Without 2nd current output									0	
With 2nd current output									1	
TAN options										
HART							SW-A001			(A)
Logbook							SW-A002			(B)
Extended logbook (Audit Trail)							SW-A003			(C)
Trace oxygen measurement							SW-A004			(D)
Current input + 2 digital inputs							SW-A005			(E)
ISM digital							SW-A006			(F)
Pfudler							SW-A007			(G)
Mounting accessories										
Pipe-mount kit							ZU 0274			
Protective hood							ZU 0737			
Panel-mount kit							ZU 0738			

Specifications

Oxy input	Input for Memosens sensors	
Operating modes	GAS	Measurement in gases
	DO	Measurement in liquids
	Temperature measurement	-20 ... +150.0 °C / -4 ... +302 °F
Display ranges Standard	Saturation (-10 ... +80 °C / +14 ... +176 °F)	0.0 ... 600.0 %
	Concentration (-10 ... +80 °C / +14 ... +176 °F)	0.00 ... 99.99 mg/l
	(Dissolved oxygen)	0.00 ... 99.99 ppm
	Volume concentration in gas	0.00 ... 99.99 %vol
Display ranges Traces (option)	Saturation (-10 ... 80°C)	0.000 ... 150.0 %
	Concentration (-10 ... 80°C) (dissolved oxygen)	0000 ... 9999 µg/l / 10.00 ... 20.00 mg/l 0000 ... 9999 ppb / 10.00 ... 20.00 ppm
	Volume concentration in gas	0000 ... 9999 ppm / 1.000 ... 50.00 %vol
Input correction	Pressure correction *	0.000 ... 9.999 bar / 999.9 kPa / 145.0 PSI manually or through current input 0(4) ... 20 mA
	Salinity correction	0.0 ... 45.0 g/kg
Sensor standardization *		
Operating modes *	AIR Automatic calibration in air	
	WTR Automatic calibration in air-saturated water	
	Product calibration	
	Zero calibration	
Calibration range Standard	Zero point	± 2 nA
	Slope	25 ... 130 nA (at +25°C/+77°F, 1013 mbar)
Calibration range Traces	Zero point	± 2 nA
	Slope	200...550 nA (at +25°C/+77°F, 1013 mbar)
Calibration timer *	Interval 0000 ... 9,999 h	
Pressure correction *	Manual 0.000 ... 9.999 bar / 999.9 kPa / 145.0 PSI	
Sensocheck/ Sensoface	Provides information on the sensor condition, evaluation of zero/slope, response time, calibration interval, wear, can be disabled	

Specifications

I input (TAN)	Current input 0/4 ... 20 mA / 50 Ω for external pressure compensation		
Start/end of scale	Configurable 0 ... 9.999 bar		
Characteristic	Linear		
Measurement error ^{1,3)}	< 1% current value + 0.1 mA		
HOLD input	Galvanically separated (optocoupler)		
Function	Switches device to HOLD mode		
Switching voltage	0 ... 2 V AC/DC	HOLD inactive	
	10 ... 30 V AC/DC	HOLD active	
CONTROL input	Galvanically separated (optocoupler)		
Function	Selecting parameter set A/B or flow measurement		
Parameter set A/B	Control input	0 ... 2 V AC/DC 10 ... 30 V AC/DC	Parameter set A Parameter set B
FLOW	Pulse input for flow measurement 0 ... 100 pulses/s		
Message	via 22 mA		
Display	00.0 ... 99.9 l/h		
Output 1	Current loop, 4 ... 20 mA, floating, protected against inverse polarity HART communication (see further below for specifications)		
Supply voltage	14 ... 30 V		
Process variable *	Saturation, concentration, salinity or temperature		
Characteristic	Linear		
Overrange *	22 mA in the case of error messages		
Output filter *	PT ₁ filter, time constant 0 ... 120 s		
Measurement error ¹⁾	< 0.25 % current value + 0.025 mA		
Start/end of scale *	Configurable within selected range		

Output 2	Current loop, 4 ... 20 mA, floating, protected against inverse polarity
Supply voltage	14 ... 30 V
Process variable *	Saturation, concentration, salinity or temperature
Characteristic	Linear
Overrange *	22 mA in the case of error messages
Output filter *	PT, filter, time constant 0 ... 120 s
Measurement error ¹⁾	< 0.25 % of current value + 0.05 mA
Start/end of scale *	Configurable within selected range
Real-time clock	Different time and date formats selectable
Power reserve	> 5 days
Display	LC display, 7-segment with icons
Main display	Character height approx. 22 mm, unit symbols approx. 14 mm
Secondary display	Character height approx. 10 mm
Text line	14 characters, 14 segments
Sensoface	3 status indicators (friendly, neutral, sad face)
Mode Indicators	meas, cal, conf, diag Further icons for configuration and messages
Alarm indication	Display blinks, red backlighting
Keypad	Keys: meas, menu, info, 4 cursor keys, enter
HART communication	HART version 6 Digital communication by FSK modulation of output current 1 Device identification, measured values, status and messages, parameter setting, calibration, records
FDA 21 CFR Part 11	Access control by editable passcodes Logbook entry and flag via HART Message and logbook entry when enclosure is opened

Specifications

Diagnostics functions

Calibration data	Calibration date, zero, slope
Device self-test	Display test, automatic memory test (RAM, FLASH, EEPROM)
Logbook	100 events with date and time
Extended logbook (TAN)	Audit Trail: 200 events with date and time

Service functions

Sensor monitor	Display of direct sensor signals
Current source	Current specifiable for output 1 and 2 (04.00 ... 22.00 mA)
Passcodes	Assigning passcodes for menu access
Factory setting	Resetting all parameters to factory setting
TAN	Enabling optionally available additional functions

Explosion protection (A2**B/X)

See Control Drawing or www.knick.de

Data retention

Parameters, calibration data, logbook > 10 years (EEPROM)

EMC

Emitted interference	Class B (residential area)
Immunity to interference	Industry EN 61326-2-3

Nominal operating conditions

Ambient temperature	-20 ... +65 °C / -4 ... +149 °F
Transport/Storage temperature	-30 ... +70 °C / -22 ... +158 °F
Relative humidity	10 ... 95% not condensing
Supply voltage	14 ... 30 V

Enclosure	Molded enclosure made of glass-reinforced PBT, PC
Mounting	Wall, pipe/post or panel mounting
Color	Gray, RAL 7001
Ingress protection	IP 67, NEMA 4X
Flammability	UL 94 V-0
Dimensions	148 mm x 148 mm
Control panel cutout	138 mm x 138 mm to DIN 43 700
Weight	Approx. 1200 g
Cable glands	3 knockouts for M20 x 1.5 cable glands 2 knockouts for NPT ½" or rigid metallic conduit
Connections	Terminals, conductor cross-section max. 2.5 mm ²

*) User-defined


1) Acc. to EN 60746, at nominal operating conditions

2) ± 1 count

3) Plus sensor error

Error Handling

Alarm condition:

- The display backlighting turns **red**
- The alarm icon  is displayed
- The complete measured-value display blinks
- “**ERR xxx**” is displayed in the lower menu line

Press the [**info**] key to view a short error text:

- The error text appears in the lower menu line
- The main display reads “**InFo**”.

Parameter errors:

Configuration data such as current range, limit values, etc are checked during the input.

If they are out of range,

- “**ERR xxx**” is displayed for 3 sec,
- the display backlighting flashes red,
- the respective maximum or minimum value is shown,
- input must be repeated.

If a faulty parameter arrives through the interface (HART),

- an error message will be displayed: “**ERR 100...199**”
- the faulty parameter can be localized by pressing the [**info**] key

Calibration errors:

If errors occur during calibration,

- an error message will be displayed

Sensoface:

If the Sensoface becomes sad,

- the display backlighting will turn purple
- the cause can be seen by pressing the **info** key
- the calibration data can be seen in the Diagnostics menu

Error Messages

Error	Info text (is displayed in case of fault when the Info key is pressed)	Problem Possible causes
ERR 99	DEVICE FAILURE	Error in factory settings EEPROM or RAM defective This error message only occurs in the case of a total defect. The device must be repaired and recalibrated at the factory.
ERR 98	CONFIGURATION ERROR	Error in configuration or calibration data Memory error in device program Configuration or calibration data defective; completely reconfigure and recalibrate the device.
ERR 97	NO MODULE INSTALLED	"MEMOSENS" not selected as sensor type
ERR 96	WRONG MODULE	"MEMOSENS" not selected as sensor type
ERR 95	SYSTEM ERROR	System error Restart required. If error still persists, send in the device for repair.
ERR 01	NO SENSOR	O₂ sensor * Sensor defective Sensor not connected Break in sensor cable
ERR 02	WRONG SENSOR	Wrong sensor *
ERR 04	SENSOR FAILURE	Failure in sensor *

Error Messages

Error	Info text (is displayed in case of fault when the Info key is pressed)	Problem Possible causes
ERR 05	CAL DATA	Error in cal data *
ERR 11	RANGE DO SATURATION	Display range violation SAT saturation CONC concentraton or GAS volume concentration
ERR 12	SENSOR CURRENT RANGE	Measuring range of sensor exceeded
ERR 13	TEMPERATURE RANGE	Temperature range violation
ERR 15	SENSOCHECK	Sensocheck
ERR 60	OUTPUT LOAD	Load error
ERR 61	OUTPUT 1 TOO LOW	Output current 1 < 3.8 mA
ERR 62	OUTPUT 1 TOO HIGH	Output current 1 > 20.5 mA
ERR 63	OUTPUT 2 TOO LOW	Output current 2 < 3.8 mA
ERR 64	OUTPUT 2 TOO HIGH	Output current 2 > 20.5 mA

* Memosens or ISM sensors

Error	Info text (is displayed in case of fault when the Info key is pressed)	Problem Possible causes
ERR 72	FLOW TOO LOW	Flow too low
ERR 73	FLOW TOO HIGH	Flow too high
ERR 105	INVALID SPAN I-INPUT	Configuration error: Current input

Sensoface

(Sensochek must have been activated during configuration.)



The smiley in the display (Sensoface) alerts to sensor problems (defective sensor, sensor wear, defective cable, maintenance request). The permitted calibration ranges and the conditions for a friendly, neutral, or sad Sensoface are summarized in the following table. Additional icons refer to the error cause.

Sensochek

Continuously monitors the sensor and its wiring.

Critical values make the Sensoface “sad” and the corresponding icon blinks:



The Sensochek message is also output as error message Err 15. The display backlighting turns red, output current 1 is set to 22 mA (when configured correspondingly).












Sensochek can be switched off during configuration (then Sensoface is also disabled).




Exception:

After a calibration a smiley is always displayed for confirmation.

Note:

The worsening of a Sensoface criterion leads to the devaluation of the Sensoface indicator (Smiley becomes “sad”). An improvement of the Sensoface indicator can only take place after calibration or removal of the sensor defect.

Display	Problem	Status
	Zero and slope	 <p>Zero and slope of the sensor are still okay. The sensor should be replaced soon.</p>
		 <p>Zero and/or slope of the sensor have reached values which no longer ensure proper calibration. Replace sensor.</p>
	Calibration timer	 <p>Over 80 % of the calibration interval has already past.</p>
		 <p>The calibration interval has been exceeded.</p>
	Sensor defect	 <p>Check the sensor and its connections (see also Err 15, Error Messages).</p>
	Response time	 <p>Sensor response time has increased. The sensor should be replaced soon. To achieve an improvement, clean the sensor and check the electrolyte and membrane.</p>
		 <p>Sensor response time has significantly increased (> 600 s, calibration aborted after 720 s) Check electrolyte and membrane, replace sensor if required.</p>

Display	Problem	Status
	Sensor wear (for digital sensors only)	<p>  Wear is over 80%. Check electrolyte and membrane. </p> <p>  Wear is at 100%. Check electrolyte and membrane, replace if required. Note: Reset the wear counter in the SERVICE - SENSOR menu when you have replaced the membrane or electrolyte. </p>
AUTOCLAVE CYCLES OVERRUN	Maximally permitted number of autoclaving cycles has been reached. Replace sensor or increment autoclaving counter.	
SIP CYCLES OVERRUN	Maximally permitted number of sterilizing cycles has been reached. Replace sensor or increment SIP counter.	
CIP CYCLES OVERRUN	Maximally permitted number of cleaning cycles has been reached. Replace sensor or increment CIP counter.	

Conformity with FDA 21 CFR Part 11

In their directive “Title 21 Code of Federal Regulations, 21 CFR Part 11, Electronic Records; Electronic Signatures” the American health agency FDA (Food and Drug Administration) regulates the production and processing of electronic documents for pharmaceutical development and production. This results in requirements for measuring devices used for corresponding applications. The following features ensure that the measuring devices of this Series meet the demands of FDA 21 CFR Part 11:

Electronic Signature – Passcodes

Access to the device functions is regulated and limited by individually adjustable codes – “Passcodes” (see SERVICE). This prevents unauthorized modification of device settings or manipulation of the measurement results. Appropriate use of these passcodes makes them suitable as electronic signature.

Audit Trail

Every (manual) change of device settings can be automatically documented. Each change is tagged with a “Configuration Change Flag”, which can be interrogated and documented using HART communication. Altered device settings or parameters can also be retrieved and documented using HART communication.

Extended logbook

Audit Trail also records function activations (CAL, CONFIG, SERVICE), some Sensoface messages (cal timer, wear) and opening of the enclosure.

Index

A

Access code assignment 95
Access codes, table 120
Accessories 98
Activating an option 95
Alarm 30
Alarm and HOLD messages 31
Alarm delay 68
Alarm settings 70
Ambulance TAN 95
Application in hazardous locations 10
Assembly 12
Audit Trail 111
Autoclaving counter: configuration 50
Autoclaving counter: description 51
Autoclaving counter: increment 94
Automatic pressure compensation 64

B

Backlighting 22
Block diagram 11

C

Calibration 78
Calibration and maintenance in the lab 74
Calibration data 89
Calibration errors 104
Calibration, general 27
Calibration medium: air/water 47
Calibration modes 79
Calibration timer, configuration 47
Calibration timer, Sensoface alert 109
CIP, cleaning cycles 49
Cleaning cycles: configuration 48
Configuration, alarm 68
Configuration, CIP/SIP settings 48
Configuration, CONTROL input 66
Configuration, correction 64
Configuration, current output 1 54

- Configuration, general 27
- Configuration, individual configuration data 41
- Configuration, measuring point 72
- Configuration, menu groups 33
- Configuration, menu structure 32
- Configuration, output current during HOLD 60
- Configuration, output current for error message or Sensoface 58
- Configuration, overview 35
- Configuration, Sensocheck 68
- Configuration, sensor 44
- Configuration, sensor verification (TAG, GROUP) 52
- Configuration, time and date 72
- Configuring the device 75
- Connection 76
- Connection example 19
- Connection to supply units 97
- CONTROL 66
- Control Drawings 3
- CONTROL input, messages 31
- Current input for pressure compensation 64
- Current output 1, configuring 54
- Current output 2, configuring 62

D

- Date and time (configuration) 72
- Date and time (usage) 73
- Date, display 87
- Device self-test 90
- Device type, display 92
- Diagnostics 88
- Diagnostics, calibration data 89
- Diagnostics, device self-test 90
- Diagnostics, general 27
- Diagnostics, sensor data 89
- Diagnostics, sensor monitor 92
- Diagnostics, version 92
- Dimensions 13
- Display 22
- Display backlighting 22

Index

Display data in Diagnostics mode 88
Display test 90
Disposal 2
Documentation 3

E

EEPROM test 90
Electronic Signature 111
Enabling an option 95
Enclosure 13
Enclosure components 12
Entering values 24
Error handling 104
Error messages 105
EU Declarations of Conformity 3
Extended logbook, Audit Trail 111
Extended logbook, diagnostics 91

F

FACE: Sensoface alert, 22 mA output current 59
FAIL: error message, 22 mA output current 59
FDA 21 CFR Part 11 111
FLASH test 90
FLOW 67
Flow measurement, alarm 70
Flow measurement, configuration 66

G

GROUP (measuring points) 73

H

HOLD, configuration 61
HOLD mode, description 29
HOLD mode, exit 29
HOLD mode, external activation 30
HOLD mode, manual activation 30
HOLD mode, output signal 29

I

Info text 105
Installation 16
Intended use 7

K

Keypad 21

L

Logbook, diagnostics 91

M

Manual pressure input 64
Measured values, display 92
Measuring mode 87
Measuring mode, overview 23
Measuring mode selection 44
Measuring points (GROUP) 73
Measuring point (TAG) 73
Measuring range 55
Memosens cable 18
Memosens, connection via RS-485 20
MemoSuite software for calibrating Memosens sensors 74
Menu structure 28
Menu structure of configuration 32
Message via CONTROL input 31
Mounting plan 13
Mounting possibilities 7

O

Operating modes 27
Operating mode, selection 24
Operating states 96
Operation and connection 74
Option request 95
Options, overview 98
Order code 98
Output current for error message (FAIL) 59
Output current for Sensoface (FACE) 59

Output current range 2, configuring 62
Output current, specify value 94
Output filter 56
Output signal during HOLD 29
Output signal during HOLD, configuration 61
Overview 8

P

Package contents 12
Package contents, documentation 3
Panel mounting 15
Parameter error 104
Parameter set A/B 33
Parameter set A/B, display 87
Parameter set A/B, individual settings 42
Parameter set selection via external signal 66
Passcodes, table 120
Pipe mounting 14
Power supply units 97
Predictive maintenance (Memosens) 75
Pressure correction 64
Pressure unit, selecting 64
Process variable for current output 1 54
Process variable for current output 2 62
Product calibration 82
Product line 98
Protective hood 14

Q

Quickstart guides 3

R

RAM test 90
Rating plates 16
Registered trademarks 119
Reset to factory settings 95
Return of products under warranty 2

S

- Safety information 10
- Safety instructions 3
- Salinity, entering 64
- Selection menu 24
- Sensocheck 108
- Sensocheck, configuration 69
- Sensoface 108
- Sensoface alerts 59
- Sensoface, troubleshooting 104
- Sensor data, display 89
- Sensor defect 109
- Sensor monitor (diagnostics) 92
- Sensor monitor (Service) 94
- Sensor verification (TAG, GROUP) 53
- Sensor wear counter, resetting (Memosens) 94
- Sensor wear, display (Memosens) 92
- Sensor wear, Sensoface alert 110
- Serial number, display 92
- Service, factory setting 95
- Service, general 27
- Service, incrementing the autoclaving counter 94
- Service mode 93
- Service, output current, specify value 94
- Service, passcode assignment 95
- Service passcode lost 95
- Service, sensor monitor 94
- Setting the passcodes 95
- Signal colors 22, 26
- Signal lines 17
- SIP, sterilization cycles 49
- Slope calibration in air 85
- Slope calibration in water 84
- Slope calibration, selecting the medium 47
- Software version, display 92
- Solution Ground - and Memosens 74
- Specifications 99
- Specific test report 3

Index

Start-up 10
Sterilization cycles: configuration 48
Supply units 97
Switchover of parameter sets A/B 34

T

Tag number, display 87
TAG (point of measurement) 73
TAN input 95
TAN options, activation 95
TAN options, overview 98
Technical data 99
Temperature probe adjustment 86
Terminal assignments 16
Terminals 16
Time and date (configuration) 72
Time and date (usage) 73
Time averaging filter 57
Time, display 87
Trademarks 119
Transaction number (TAN) 95

U

User interface 21

W

Weather protector 14
Wiring 17
Wiring example 19
Wiring, power supply units 97

Z

Zero calibration 80

The following names are registered trademarks. For practical reasons they are shown without trademark symbol in this manual.

Stratos®

Sensocheck®

Sensoface®

Calimatic®

GainCheck®

InPro® is a registered trademark of Mettler-Toledo AG.

ISM® is a registered trademark of Mettler-Toledo AG.

Memosens® is a registered trademark of Endress+Hauser Conducta GmbH and Knick Elektronische Messgeräte GmbH & Co. KG.

HART® is a registered trademark of the HART Communication Foundation.

Passcodes

In the SERVICE – CODES menu you can assign passcodes to protect the access to certain functions.

Mode of operation	Passcode
Service (SERVICE)	5555
Diagnostics (DIAG)	
HOLD mode	
Calibration (CAL)	
Configuration (CONF)	

Knick

Elektronische Messgeräte GmbH & Co. KG

Beuckestraße 22

14163 Berlin

Germany

Phone: +49 30 80191-0

Fax: +49 30 80191-200

Web: www.knick.de

Email: info@knick.de



099467

Stratos Pro A2.. MSOxy: O₂ Measurement with Memosens

TA-212.145-MS-KNEN05

20170831

Software version: 3.x